

BENEFITS

The NGC 8209, the C9+ Natural Gas Chromatograph performs on-site natural gas analysis and heating value computation using an extended analysis. On-line chromatograph techniques are used to provide N2 through C6+ data while a third column train is used to separate the C6+ fraction. The NGC 8209 utilizes the modular and scaleable XSeries software framework to integrate data from a third



analysis train into the standard C6+ analysis of the Natural Gas. The extra chromatographic information is provided as NC6's, NC7's, NC8's and C9+ to provide this "extended analysis". Heating value (CV), Wobbe, Relative Density (SG) and other calculations are performed using the combined analysis data in a similar manner to the NGC 8206. Hydrocarbon Dew Point (HCDP) and Speed of Sound (SOS) calculations are available options. A single computer controller seamlessly processes all this data for various outputs. It also handles the stream switching and the timing for the sample.

Incorporating a state-of-the-art built-in 32 bit digital controller, three electronic carrier pressure regulators, oven-mounted sensors and advanced low-noise digital electronics, the NGC 8209 performs with unparalleled repeatability and sensitivity.

The NGC 8209 provides custody transfer/metrology quality Chromatography for heating value and composition measurement. It provides the user with a GC that is lower in cost, easier to install and commission, and less costly to operate.

STANDARD FEATURES

- Modular design includes:
- Three analysis trains, two for N2 through C6+ and one for the C6 through C9+
- Modular software – application based plug-in software modules
- Manifold modules
- Analysis sections contain stream selection solenoids, temperature and pressure regulation, 32 bit digital detector electronics, replaceable column / valve modules and a low power 32 bit digital controller, using Windows CE® (internal to GC unit)
- Microsoft® Windows® 2000 or XP based man-machine interface software (PCCU_NGC)
- Lithium battery-backed RAM
- Two remote serial digital communications ports; one local port (USB Client)
- One USB Host and one Ethernet port
- Comprehensive diagnostics and wizards available to users
- Three-level security for user access control (Read only, Operate and Read/Write)
- Audit-quality historical data; date and time stamped
- Standard Calculations; US and SI:
 - ◊ Heating value
 - ◊ Relative density
 - ◊ GPM
 - ◊ Wobbe
 - ◊ Methane-number
- Auto-start cycle automatically after power failure:
 - ◊ Stabilizes oven temperature
 - ◊ Confirms modules' functions
 - ◊ Checks for operational alarms
 - ◊ Returns to pipeline streams
- Operational alarms available with each analysis cycle.
- Detectors - constant temperature, glass encapsulated thermister beads for rugged service and long life. Will not burn out on loss of carrier.
- 10 port valves have no moving metal parts in each analysis unit
- Low utility usage - low-power, low-carrier, no instrument air required

- On demand or scheduled automatic calibration and diagnostics
- Continuous monitoring for alarms

STANDARD OPTIONS

- H2S measurement from 0.02% and higher
- Sample Conditioning Modules
- On board digital 1/4 VGA display with multiple screen access
- Calculation packages (eg, Hydrocarbon Dew point via SRK and Peng-Robinson, including: 4 pressures and the Cricondentherm)
- Integral gas flow tube calculations (e.g. Orifice or turbine meter calculations)
- SD memory cards for raw chromatogram storage
- Feed-Through heater for colder operations or high dew point gas sampling

DESCRIPTION

A natural gas sample is extracted from a flowing pipeline, transported to the analyzer, processed for particle removal and phase integrity, injected onto the three sets of chromatographic columns where component separation and peak detection occurs.

The NGC 8209 analyzes each sample utilizing established chromatographic techniques. The resulting information consists of mole percent values for the following:

"Air" (Contains N₂, CO, Ar, and O₂)

C₁ CO₂ C₂ C₃ IC₄

NC₄ NeoC₅ IC₅ NC₅ C₆'s C₇'s C₈'s C₉+

Using process chromatographic techniques, the columns are back flushed so that the NGC 8209 measures a C₃+, C₆+, and a C₉+ peak. The rest of the analyzed components are carried through the columns and the detectors where integration takes place. Composition results and calculated values are then stored in memory and communicated to other devices as needed. All of these values as well as composition are available on various Modbus communication protocols.

INSTALLATION

The NGC 8209 is a weatherproof device designed for installation "on the pipe" near to the sampling point. This means it is acceptable to mount outside - in a temperature range of 0°F to 131°F (-18°C to 55°C), onto a pipeline with 2" to 12" pipe sizes or with an optional pole mount configuration. A cold weather

enclosure is also available if ambient conditions are below either the sampled gas dew point or the operational specifications of the unit. If ambient temperatures are expected to exceed 131°F (55°C) we recommend installing a sun shade.

SAMPLE SYSTEM

The integral stream selector for the NGC 8209 allows sampling up to four (4) different natural gas streams. Up to two of these sample streams can be designated as the "calibration/validation sample". Optional sample conditioning modules are available to address natural gas streams that need additional filtering and "speed loops" to reduce sample transport lag times.

SAMPLE PROBE

Totalflow recommends the use of a sample probe to obtain a representative sample of the flowing gas stream. Two brands of optional sample probes are available from Totalflow and are specifically designed to require no power and avoid sample probe regulator icing. An electrically heated probe is also available.


OPERATOR INTERFACES

Functional setup and operation of the NGC 8209 is accomplished by using a graphical user interface software package called PCCU_NGC (supplied with each unit) operating on a laptop PC in a Microsoft® Windows® 2000 or XP environment. PCCU_NGC, software designed specifically for the NGC 8209, provides a powerful tool for operations, diagnostics, and downstream data handling. The PC can be directly connected to the NGC 8209 via an RS-232, USB, or Ethernet connection, or indirectly by remote telemetry (phone modem, radio, cell phone, satellite, etc.). The user is prompted through push-buttons, drop-down boxes, wizards, and dialog boxes for setup, operations, data collection and monitoring.

In addition, the unit has an optional 1/4 VGA interactive display screen allowing the user access to basic analysis data and perform basic operations.

MAINTENANCE

The NGC 8209 was designed from the ground up to be maintained by personnel with little or no prior knowledge of Gas Chromatography. Both hardware

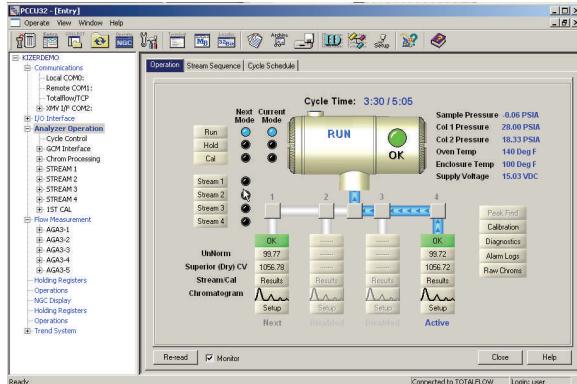

and software are designed to provide low maintenance through easily replaceable electro-mechanical modules such as:

- NGC Termination Panel
- NGC Analytical Module, an easily removable Chromatograph subassembly, containing; NGC Manifold, Stream Selector Solenoid Valves, GC valve assembly, Multiple Electronic Carrier Pressure Regulator Valves, Chromatograph Pilot Valve, and the NGC Analytical Processor.
- NGC Feed-Through (with optional heater)
- Sample Conditioning Module (SCM) (optional)
- NGC Controller, (32 bit Processor)
- NGC 1/4 VGA Display (Optional)

Other Maintenance Support Features:

- Intuitive Local Operator Interface (PCCU_NGC) running Microsoft® Windows® 2000 or XP
- Diagnostic software and wizards (future) for maintenance
- Diagnostic file output system for e-mail support (future)
- Digitized detector output (chromatogram) to PCCU_NGC
- Remote or local operation of PCCU_NGC
- Quick Start guide, Start up manual and Start up video (future)

HISTORICAL DATA

The NGC 8209 is designed to retain historical data. This data can be used for custody transfer needs, verify transmitter operation over time, and provide a limited data backup for communication link reliability.

The user is allowed to configure the period of the data retained by the NGC 8209 via the Operator Interface.

The default* memory configuration provides the most recent 480 analysis cycles containing:


- Normalized components
- Un-normalized components
- Ideal Btu/CV
- Real Btu (wet and dry) / CV (superior and inferior)
- Relative Density (Specific Gravity)
- Density
- GPM
- Wobbe index
- HCDP
- Alarms

Stream averages for the (default*) 840 last hours, 35 last days and the most recent last month analyses.

Operational Parameters for the (default*) last 480 cycles (Diagnostics Report):

- Selected peak times
- Selected peak areas
- Ideal Btu/CV
- Carrier regulator pressure
- Oven temperature
- Ambient temperature
- Sample pressure
- Detector noise values
- Detector balance values
- Audit logs (Default*)
- Last 480 alarms
- Last 480 events

Data retained by the NGC 8209 can be collected via a remote communication link or by the laptop PC local operator interface PCCU_NGC.

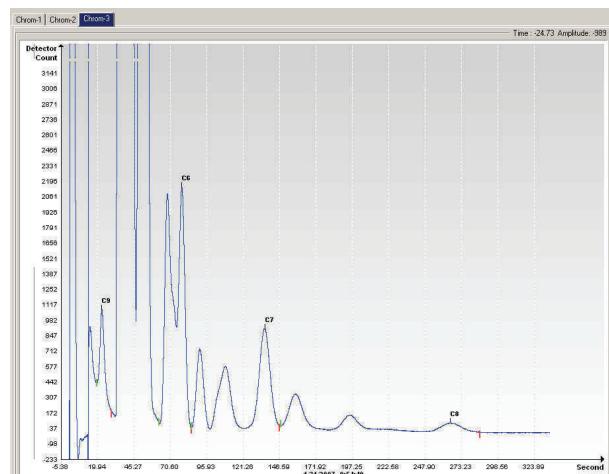

SPECIFICATIONS

- Designed for Pipeline-Quality Natural Gas containing 800 to 1500 Btu per standard cubic foot (29.8 to 55.9 megajoules/meter³) with less than 100 PPM H₂S
- Calculations Per: GPA 2172-96 (Z by AGA 8 or single virial summation) and 2145-03 (rev 1), ISO 6976-95; The determination of the composition per ISO 6974; The determination of the calorific value, relative density and of Wobbe number per ISO 6976; The determination of the compressibility factor per ISO 12213; in the future: ASTM D 3588, GOST and ISO mass
- Meet or exceeds GPA 2261-99 for linearity
- Four stream capability. Manual calibration required with 4 sample streams.
- Single auto calibration stream and 3 sample streams, or a max of 2 auto calibration streams and 2 sample streams.

Specifications	
Dimensions	22.58" wide (57.35 cm) × 17.1" deep (43.43 cm) × 22.50" high (57.15 cm)
Weight	Approximately 50 lb. (22 Kg) Shipping Weight: 94 lb. (45 Kg)
Weatherproof Construction	NEMA/Type-4X/IP 56, aluminum alloy with white polyester powder coating
Power Consumption	Nominal operation @ 0°F (-18°C) = 14 Watts; (1300 mA) Start up @ less than 6 amps (90 Watts @ 15 VDC)
Carrier Gas	Helium (consumption rate <40 cc/minute during analysis cycle)
Analysis Time	Approximately six (6) minutes; cycles may be scheduled by user
Repeatability	±0.25 Btu @ 1,000 Btu (±0.025%) at a fixed temperature ±0.5 Btu @ 1,000 Btu (±0.05%) over temperature range
Temperature Range Temperature Range (Storage) with Cold Weather Enclosure	0°F to 131°F (-18°C to 55°C) -22°F to +140°F (-30°C to 60°C) -40°F to +131°F (-40°C to 55°C)
Moisture	95% Relative Humidity Non-Condensing
Supply Voltage	10.5 to 16 volts DC Or 21 to 28 VDC as an option
Certifications	NEC & CEC Class I, Div. 1, Groups B, C and D, T6 CFR 47, Part 15 CE: ATEX II 2G : Ex d, IIB+H ₂ T6; Class I, Zone 1 EMC - EMI/RFI EN 55022, EN 61000-6-1, EN 61000-4-2, 4-3, 4-4, 4-6, 4-8 CISPR 22-2004 IECEx Ex d IIB + H2 T6; Class I, Zone 1
Communications supported	Two serial digital ports, software selectable for RS232, RS485, or RS422 One Man-Machine Interface (USB Slave) One USB host One Ethernet Port
Protocols supported	Totalflow Remote / Local MMI Totalflow / TCP Modbus / TCP Server Modbus / TCP Client Modbus ASCII or RTU (Modicon, WordSwap, or Danalyzer 2251) Marquis Protocol (future)

AVAILABLE ACCESSORIES

- 120/240 VAC to 12VDC power supply
- 120/240 VAC to 24VDC power supply
- Pole or pipeline mounting kits
- Cold weather enclosure (also available in pipe mount configuration)
- Cold weather thermal jacket (future)
- Modular Sample System Conditioner options for
 - Non-pipeline quality natural gas sample
 - Up to 450 LC/min speed loops
- Probes
 - Temperature compensating fixed
 - Temperature compensating retractable
 - Liquid rejection
 - Electrically heated, retractable
- Regulators (carrier and calibration blend)
- Start-up calibration/validation gas sample ($\pm 2\%$ blend)
- Carrier Gas: 99.995% pure helium (chromatographic grade)
- SD memory card, various up to 1Gig
- Export crating
- Tool kit
- Welker and A+ Corp. liquid shut-offs
- Various maintenance kits
- Customer Factory Acceptance Test (FAT)

Note on Linearity of C6 through C9+:

Extensive linearity testing is usually done to prove the design of a GC. This has been done for the NGC 8206 and the results can be obtained in another datasheet. It is, however, doubtful that the same data could be obtained for the "extended analysis" fraction, that is, the components beyond C6 and up to C9+.

The reasons for this are as follows:

- The wide concentration ranges needed to produce the linearity data will themselves prevent building stable calibration blends. When blends with more than 1000 ppm (0.1 Mol %) of any of the C6, C7, C8, and C9+ components are added to a blend, the Hydrocarbon Dew Point (HDP) of that blend will tend to make it become a liquid unless kept and sampled at a high temperature. Greater than 1000 ppm of C6, C7, C8, or C9 increases the HDP to such a point the mixture would have to be heated beyond 120F-140F to keep the mixture a gas. This increases the difficulty of keeping or sampling from the needed blends.
- The accuracy of a gravimetric calibration blend at these very low mol % levels drops off significantly due to the very small weights of the gases added. This leads to a much greater error in the resulting mol % of each component and therefore in the accuracy of the blend. This inaccuracy tends to make the generation of the detector response curve meaningless.

However, the usable linear range of the detectors is quite wide at the reasonable operating concentrations found in these heavier fractions in comparison to the possible variations in blend concentrations. So the NGC linearity will likely exceed the real world requirements.

Power and Productivity
for a Better World.™

www.abb.com/totalflow

www.abb.us

www.abb.com



ABB Inc.
Totalflow Products
 7051 Industrial Blvd.
 Bartlesville, OK 74006
 Tel: (918) 338-4888
 Fax: (918) 338-4699
 (800) 442-3097

ABB Inc.
Totalflow Products
 3010 Briarpark Dr., Ste. 200
 Houston, TX 77042
 Tel: (713) 821-8909
 Fax: (713) 821-3521

For more information,
 please contact your
 local ABB Totalflow
 representative or visit
 our website.