



Ranibizumab ELISA

REF : KBI1029

Ver 3.0

RUO

Enzyme Immunoassay for the quantitative determination of Ranibizumab in serum, plasma and cell culture supernatant

RUO	For Research Use	REF	Catalog Number
	Store At	LOT	Batch Code
	Manufactured By		Biological Risk
	Expiry Date		Consult Operating Instructions

For Research Use Only. Purchase does not include or carry the right to resell or transfer this product either as a stand-alone product or as a component of another product. Any use of this product other than the permitted use without the express written authorization of Eagle Biosciences, Inc. is strictly prohibited.



REF KBI1029

96 tests



Eagle Biosciences

20A NW BLVD., Suite 112
Nashua, NH 03063
Phone: +1 (617) 419-2019
Fax: +1 (617) 419-1110
Info@eaglebio.com

Introduction:

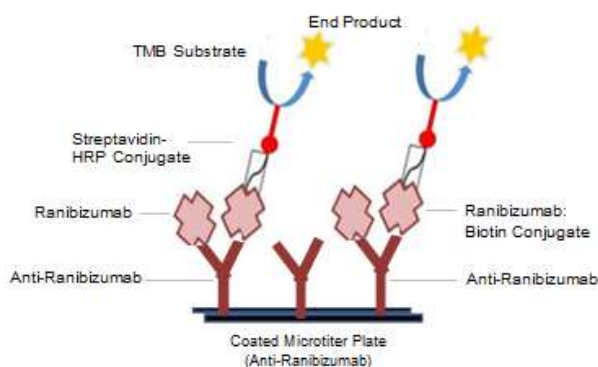
Ranibizumab (Lucentis) is a recombinant humanized IgG1 monoclonal antibody fragment that binds to and inhibits vascular endothelial growth factor A (VEGF-A). VEGF is a biochemical signal protein that promotes angiogenesis throughout the body and in the eye. Through binding to VEGF-A, ranibizumab interrupts the interaction of VEGF with its receptors, and thus prevents the subsequent growth of new blood vessels.

Intended Use:

The Eagle Biosciences Ranibizumab ELISA is used as an analytical tool for quantitative determination of Ranibizumab in serum, plasma and cell culture supernatant.

Principle:

The method employs the competitive enzyme immunoassay technique. Antibodies to Ranibizumab are pre-coated onto microwells. Samples or Standards and Ranibizumab-Biotin Conjugate are pipetted into microwells and human Ranibizumab present in the sample or standard will compete with Ranibizumab-Biotin Conjugate and bound by the capture antibody. After washing microwells, HRP conjugate is pipetted and incubated. Free HRP conjugate will be removed by washing cycle. The ready to use substrate solution (TMB) is added to microwells and color develops inversely proportional to the amount of Ranibizumab in the sample. Color development is then stopped by addition of stop solution. Absorbance is measured at 450 nm.

**Materials Provided:**

1. Anti-Ranibizumab Coated Microtiter Plate (12x8 wells) – 1 no
2. Ranibizumab Standard, (1.0 ml/vial) – 0, 1.25, 2.5, 5, 10, 20, 40 and 80 ng/ml
3. Ranibizumab: Biotin Conjugate – 6 ml
4. Streptavidin: HRP Conjugate – 12 ml
5. Sample Diluent – 12 ml
6. Wash Buffer (20X) – 30 ml
7. TMB Substrate – 12 ml
8. Stop Solution – 12 ml
9. Instruction Manual

Materials to be provided by the End-User:

1. Microtiter Plate Reader able to measure absorbance at 450 nm.
2. Adjustable pipettes and multichannel pipettor to measure volumes ranging from 25µl to 1000µl
3. Deionized (DI) water
4. Wash bottle or automated microplate washer
5. Semi-Log graph paper or software for data analysis
6. Timer
7. Absorbent Paper

Handling/Storage:

1. All reagents should be stored at 2°C to 8°C for stability.
2. All the reagents and wash solutions should be used within 12 months from manufacturing date.
3. Before using, bring all components to room temperature (18-25°C). Upon assay completion ensure all components of the kit are returned to appropriate storage conditions.
4. The Substrate is light-sensitive and should be protected from direct sunlight or UV sources.

Health Hazard Warnings:

1. Reagents that contain preservatives may be harmful if ingested, inhaled or absorbed through the skin.
2. For Research Use Only.



Sample Preparation and Storage:

Blood is taken by venipuncture. Serum is separated after clotting by centrifugation. Plasma can be used, too. Lipaemic, hemolytic or contaminated samples should not be run. Repeated freezing and thawing should be avoided. If samples are to be used for several assays, initially aliquot samples and keep at -20°C.

For Cell Culture Supernatant – If necessary, centrifuge to remove debris prior to analysis. Samples can be stored at -20°C or -80°C. Avoid repeated freeze-thaw cycles.

Preparation Before Use:

Allow samples to reach room temperature prior to assay. Take care to agitate patient samples gently in order to ensure homogeneity.

Test Sample preparation - Samples have to be diluted 1:500 to 1:1000 (v/v), e.g. for 1:500 (1 µl sample + 499 µl sample diluent) prior to assay. The samples may be kept at 2 - 8°C for up to three days. Long-term storage requires -20°C.

Reagent Preparation (all reagents should be diluted immediately prior to use):

1. Label any aliquots made with the kit Lot No and Expiration date and store it at appropriate conditions mentioned.
2. Bring all reagents to Room temperature before use.
3. To make Wash Buffer (1X); dilute 50 ml of 20X Wash Buffer in 950 ml of DI water.

Procedural Notes:

1. In order to achieve good assay reproducibility and sensitivity, proper washing of the plates to remove excess un-reacted reagents is essential.
2. High Dose Hook Effect may be observed in samples with very high concentrations of Ranibizumab. High Dose Hook Effect is due to excess of antibody for very high concentrations of Ranibizumab present in the sample. High Dose Hook effect is most likely encountered from samples early in the purification process. If Hook Effect is possible, the samples to be assayed should be diluted with a compatible diluent. Thus if the Ranibizumab concentration of the undiluted sample is less than the diluted sample, this may be indicative of the Hook Effect.
3. Avoid assay of Samples containing sodium azide (NaN_3), as it could destroy the HRP activity resulting in under-estimation of the amount of Ranibizumab.
4. It is recommended that all Standards and Samples be assayed in duplicates.
5. Maintain a repetitive timing sequence from well to well for all the steps to ensure that the incubation timings are same for each well.
6. If the Substrate has a distinct blue color prior to use it may have been contaminated and use of such substrate can lead to compromisation of the sensitivity of the assay.
7. The plates should be read within 30 minutes after adding the Stop Solution.
8. Make a work list in order to identify the location of Standards and Samples.

Assay Procedure:

1. It is strongly recommended that all Controls and Samples be run in duplicates or triplicates. A standard curve is required for each assay. All steps must be performed at 37°C

2. Add **100 µl** of **Standards** or **Samples** into the respective wells.
3. Cover the plate and incubate for 120 minutes at 37°C.
4. Pipette **50 µl** of **Ranibizumab: Biotin Conjugate** into each well.
5. Cover the plate and incubate for 60 minutes at 37°C
6. Aspirate and wash plate 4 times with **Wash Buffer (1X)** and blot residual buffer by firmly tapping plate upside down on absorbent paper. Wipe of any liquid from the bottom outside of the microtiter wells as any residue can interfere in the reading step.
7. Add **100 µl** of **Streptavidin: HRP Conjugate** into each well.
8. Aspirate and wash plate 4 times with **Wash Buffer (1X)** and blot residual buffer by firmly tapping plate upside down on absorbent paper. Wipe of any liquid from the bottom outside of the microtiter wells as any residue can interfere in the reading step.
9. Add **100 µl** of **TMB Substrate** in each well.
10. Incubate the plate at 37°C for 60 minutes in dark. DO NOT SHAKE or else it may result in higher backgrounds and worse precision. Positive wells should turn bluish in color.
11. Pipette out **100 µl** of **Stop Solution**. Wells should turn from blue to yellow in color.
12. Read the absorbance at 450 nm with a microplate reader.

Calculation of Results:

Determine the Mean Absorbance for each set of duplicate or triplicate Standards and Samples. Using Semi-Log graph paper, plot the average value (absorbance 450nm) of each standard on the Y-axis versus the corresponding concentration of the standards on the X-axis. Draw the best fit curve through the standard points. To determine the unknown Ranibizumab concentrations, find the unknown's Mean Absorbance value on the Y-axis and draw a horizontal line to the standard curve. At the point of intersection, draw a vertical line to the X-axis and read the Ranibizumab Concentration. If samples were diluted, multiply by the appropriate dilution factor. Software which is able to generate a cubic spline curve-fit is best recommended for automated results.

Note:

It is recommended to repeat the assay at a different dilution factor in the following cases:

- If the sample absorbance value is below the first standard.
- If the absorbance value is equivalent or higher than the 80 ng/ml standard.

Quality Control:

It is recommended that for each laboratory assay appropriate quality control samples in each run to be used to ensure that all reagents and procedures are correct.

Performance Characteristics of the Kit:

This kit has been validated as per EMA/FDA guidelines in line with ICH Code for Harmonization of Biological Assays.

Sensitivity:

Limit Of Detection: It is defined as the lowest detectable concentration corresponding to a signal of Mean of '0' standard plus 2* SD.

10 replicates of '0' standards were evaluated and the LOD was found to be less than 1.25 ng/ml

Linearity:

Standards provided in the kit will be used for measuring the linearity range of Ranibizumab present in matrix.

Precision:

Precision is defined as the percent coefficient of variation (%CV) i.e. standard deviation divided by the mean and multiplied by 100. Assay precision was determined by both intra (n=5 assays) and inter assay (n=5 assays) reproducibility on two pools with low (1.25 ng/ml), medium (10 ng/ml) and high (80 ng/ml) concentrations. While actual precision may vary from laboratory to laboratory and technician to technician, it is recommended that all operators achieve precision below these design goals before reporting results.

Pool	Intra Assay %CV	Inter Assay %CV
Low	<10%	<10%
Medium	<5%	<5%
High	<5%	<5%

Limitations of Method

Healthy individuals should be tested negative by the Ranibizumab. This kit is for research use only and should not be used as a diagnostic tool.

Safety Precautions:

- **This kit is for research only.** Follow the working instructions carefully.
- The expiration dates stated on the kit are to be observed. The same relates to the stability stated for reagents
- Do not use or mix reagents from different lots.
- Do not use reagents from other manufacturers.
- Avoid time shift during pipetting of reagents.
- All reagents should be kept in the original shipping container.
- Some of the reagents contain small amount of sodium azide (< 0.1 % w/w) as preservative. They must not be swallowed or allowed to come into contact with skin or mucosa.
- Source materials maybe derived from human body fluids or organs used in the preparation of this kit were tested and found negative for HBsAg and HIV as well as for HCV antibodies. However, no known test guarantees the absence of such viral agents. Therefore, handle all components and all patient samples as if potentially hazardous.
- Since the kit contains potentially hazardous materials, the following precautions should be observed
 - Do not smoke, eat or drink while handling kit material
 - Always use protective gloves
 - Never pipette material by mouth
 - Wipe up spills promptly, washing the affected surface thoroughly with a decontaminant.
- In any case GLP should be applied with all general and individual regulations to the use of this kit.

**References:**

Serum and Plasma Vascular Endothelial Growth Factor Concentrations Before and After Intravitreal Injection of Aflibercept or Ranibizumab for Age-Related Macular Degeneration...Wang X, Sawada T, Sawada O....Am J Ophthalmol...2014...Elsevier

Ranibizumab and aflibercept:intraocular pharmacokinetics and their effects on aqueous VEGF level in vitrectomized and nonvitrectomized macaque eyes...Niwa Y, Kakinoki M, Sawada T, Wang X, Ohji M...Invest Ophthalmol Vis Sci...2015...ARVO

Pharmacokinetics of Ranibizumab after Intravitreal Administration in Patients with Retinal Vein Occlusion or Diabetic Macular Edema...Yi Zhang, Zhenling Yao, Nitin Kaila, Peter Kuebler...Ophthalmology...2014...American Academy of Ophthalmology

Evaluation of fluorophotometry to assess the vitreal pharmacokinetics of protein therapeutics... Dickmann LJ, Yip V, Li C...Invest Ophthalmol Vis Sci...2015... ARVO

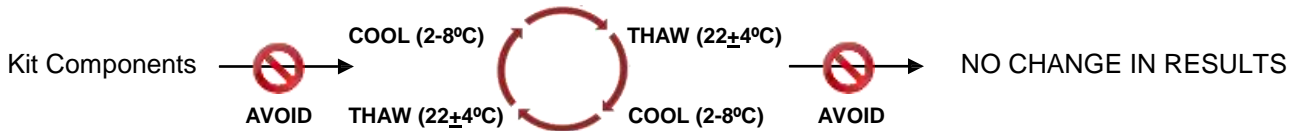
Vascular endothelial growth factor plasma levels before and after treatment of retinopathy of prematurity with ranibizumab...Graefes Ying Zhou, Yanrong Jiang, Yujing Bai, Jing Wen, Li Chen...Arch Clin Exp Ophthalmol...2016... Springer

SCHEMATIC ASSAY PROCEDURE



1. Remove all components, 30 minutes before adding into the assay plate.





2. Avoid repeated cool-thaw of the components as there will be a loss of activity and this can affect the results.



3.  Pipette **150µl Standards / Samples** into the respective wells



4. Cover plate  and incubate for  at 37°C


5.  Pipette **50µl Ranibizumab:Biotin Conjugate** into each well

6. Cover plate  and incubate for  at 37°C



7.  Aspirate and wash wells 5 times with **Wash Buffer (1X)**

8.  Pipette **100µl Streptavidin-HRP Conjugate** into each well

9. Cover plate  and incubate for  at 37°C

10.  Aspirate and wash wells 5 times with **Wash Buffer (1X)**

11.  Pipette **100µl TMB Substrate** into each well

12. Cover plate  and incubate for  at 37°C.

13.  Pipette **100µl Stop Solution** into each well.

14. Read absorbance at 450nm with a  microplate reader within  of stopping reaction.

Typical Example of a Work List

Well #	Contents	Absorbance at 450nm	Mean Absorbance	ng/ml Ranibizumab equivalent
1A 2A	zero std zero std			
1B 2B	1.25 ng/ml 1.25 ng/ml			
1C 2C	2.5 ng/ml 2.5 ng/ml			
1D 2D	5 ng/ml 5 ng/ml			
1E 2E	10 ng/ml 10 ng/ml			
1F 2F	20 ng/ml 20 ng/ml			
1G 2G	40 ng/ml 40 ng/ml			
1H 2H	80 ng/ml 80 ng/ml			
3A 4A	Sample			
3B 4B	Sample			

LIMITED WARRANTY

Eagle Biosciences, Inc. warrants its Product(s) to operate or perform substantially in conformance with its specifications, as set forth in the accompanying package insert. This warranty is expressly limited to the refund of the price of any defective Product or the replacement of any defective Product with new Product. This warranty applies only when the Buyer gives written notice to the Eagle Biosciences within the expiration period of the Product(s) by the Buyer. In addition, Eagle Biosciences has no obligation to replace Product(s) as result of a) Buyer negligence, fault, or misuse, b) improper use, c) improper storage and handling, d) intentional damage, or e) event of force majeure, acts of God, or accident.

Eagle Biosciences makes no warranties, either expressed or implied, except as provided herein, including without limitation thereof, warranties as to marketability, merchantability, fitness for a particular purpose or use, or noninfringement of any intellectual property rights. In no event shall the company be liable for any indirect, incidental, or consequential damages of any nature, or losses or expenses resulting from any defective product or the use of any product. Product(s) may not be resold, modified, or altered for resale without prior written approval from Eagle Biosciences, Inc.

For further information about this kit, its application or the procedures in this kit insert, please contact the Technical Service Team at Eagle Biosciences, Inc. at info@eaglebio.com or at 866-411-8023.

THANK YOU FOR USING EAGLE BIOSCIENCES!