



















## **Technical Information**

## Tank Side Monitor NRF590

Inventory Control

Field device for tank sensor operation and monitoring and for integration into inventory control systems Software Version 02.04



#### Application

The Tank Side Monitor NRF590 is a sensor integration and monitoring unit for bulk storage tank gauging applications.

It can be used with Micropilot radar or Proservo level gauges and can be combined with other HART compatible devices.

The Tank Side Monitor offers the following functions:

- intrinsically safe (i.s.) power supply of the connected
- parametrization of the connected devices
- display of the measured values
- tank calculations for accurate correction of the tank distortions

#### Features and benefits

- I.s. power supply and communication for Micropilot and Levelflex level radars
- Connects up to 6 HART devices via i.s. 2 wire, for example Prothermo for average temperature measurement and Cerabar/Deltabar for HTMS density applications
- Backlit graphical LCD display; operation via 3 optical keys (touch control)
- User-friendly operating menu (multi-lingual)
- Interfaces to the tank inventory system Tankvision
- Provides communication to PLC, DCS and SCADA
- Various industry standard communication protocols, including
  - Sakura V1
  - EIA-485 Modbus
  - Whessoematic WM550
  - BPM (compatible with Enraf systems)
- Approved for use in explosion hazardous areas
- Weights & Measure-approved for use in custody transfer applications



## **Table of Contents**

Function and system design
Application
Operating principle
System Integration (typical example)
HART interface
Power supply for HART instruments
Operation of HART instruments
Typical Tank calculations
Corrections
Overfill protection
Inputs and outputs8
Non IS inputs and outputs
Fieldbus Protocols
Values transmitted by the Field Protocols
Technical data of the non-IS inputs and outputs
Technical Data of the IS inputs and outputs
Technical Ball of the le hipate and outpute
Auxiliary energy13
AC supply
DC supply
Power consumption
Fuse
Grounding
Floring compation was a terminal.
Electrical connection - non-i.s. terminals
Terminal assignment of the field protocol/host side
Terminal assignment of the field protocol/host side
Terminal assignment of the field protocol/host side
Terminal assignment of the field protocol/host side
Terminal assignment of the field protocol/host side
Terminal assignment of the field protocol/host side
Terminal assignment of the field protocol/host side
Terminal assignment of the field protocol/host side
Terminal assignment of the field protocol/host side
Terminal assignment of the field protocol/host side
Terminal assignment of the field protocol/host side
Terminal assignment of the field protocol/host side 14 Connection of the field protocols 15 Grounding of the fieldbus screen 15 Connection of the auxiliary energy 15 Connection of the non-i.s. 4 to 20 mA analogue input 16 Connection of the non-i.s. 4 to 20 mA analogue output 16 Connection of the discrete in and output 16  Electrical connection - i.s. terminals 17 Terminal assignment 17 Connection of HART instruments 18
Terminal assignment of the field protocol/host side
Terminal assignment of the field protocol/host side 14 Connection of the field protocols 15 Grounding of the fieldbus screen 15 Connection of the auxiliary energy 15 Connection of the non-i.s. 4 to 20 mA analogue input 16 Connection of the non-i.s. 4 to 20 mA analogue output 16 Connection of the discrete in and output 16  Electrical connection - i.s. terminals 17 Terminal assignment 17 Connection of HART instruments 18 Spot RTD 18
Terminal assignment of the field protocol/host side 14 Connection of the field protocols 15 Grounding of the fieldbus screen 15 Connection of the auxiliary energy 15 Connection of the non-i.s. 4 to 20 mA analogue input 16 Connection of the non-i.s. 4 to 20 mA analogue output 16 Connection of the discrete in and output 16 Connection of the discrete in and output 16  Electrical connection - i.s. terminals 17 Terminal assignment 17 Connection of HART instruments 18 Spot RTD 18
Terminal assignment of the field protocol/host side 14 Connection of the field protocols 15 Grounding of the fieldbus screen 15 Connection of the auxiliary energy 15 Connection of the non-i.s. 4 to 20 mA analogue input 16 Connection of the non-i.s. 4 to 20 mA analogue output 16 Connection of the discrete in and output 16  Electrical connection - i.s. terminals 17 Terminal assignment 17 Connection of HART instruments 18 Spot RTD 18  Performance characteristics 19 Accuracy 19
Terminal assignment of the field protocol/host side 14 Connection of the field protocols 15 Grounding of the fieldbus screen 15 Connection of the auxiliary energy 15 Connection of the non-i.s. 4 to 20 mA analogue input 16 Connection of the non-i.s. 4 to 20 mA analogue output 16 Connection of the discrete in and output 16  Electrical connection - i.s. terminals 17 Terminal assignment 17 Connection of HART instruments 18 Spot RTD 18  Performance characteristics 19 Accuracy 19 Resolution 19
Terminal assignment of the field protocol/host side 14 Connection of the field protocols 15 Grounding of the fieldbus screen 15 Connection of the auxiliary energy 15 Connection of the non-i.s. 4 to 20 mA analogue input 16 Connection of the non-i.s. 4 to 20 mA analogue output 16 Connection of the discrete in and output 16  Electrical connection - i.s. terminals 17 Terminal assignment 17 Connection of HART instruments 18 Spot RTD 18  Performance characteristics 19 Accuracy 19
Terminal assignment of the field protocol/host side 14 Connection of the field protocols 15 Grounding of the fieldbus screen 15 Connection of the auxiliary energy 15 Connection of the non-i.s. 4 to 20 mA analogue input 16 Connection of the non-i.s. 4 to 20 mA analogue output 16 Connection of the discrete in and output 16  Electrical connection - i.s. terminals 17 Terminal assignment 17 Connection of HART instruments 18 Spot RTD 18  Performance characteristics 19 Accuracy 19 Resolution 19
Terminal assignment of the field protocol/host side 14 Connection of the field protocols 15 Grounding of the fieldbus screen 15 Connection of the auxiliary energy 15 Connection of the non-i.s. 4 to 20 mA analogue input 16 Connection of the non-i.s. 4 to 20 mA analogue output 16 Connection of the discrete in and output 16 Connection of the discrete in and output 16  Electrical connection - i.s. terminals 17 Terminal assignment 17 Connection of HART instruments 18 Spot RTD 18  Performance characteristics 19 Accuracy 19 Resolution 19 Scan time 19  Installation conditions 20 Wall mounting 20
Terminal assignment of the field protocol/host side 14 Connection of the field protocols 15 Grounding of the fieldbus screen 15 Connection of the auxiliary energy 15 Connection of the non-i.s. 4 to 20 mA analogue input 16 Connection of the non-i.s. 4 to 20 mA analogue output 16 Connection of the discrete in and output 16  Electrical connection - i.s. terminals 17 Terminal assignment 17 Connection of HART instruments 18 Spot RTD 18  Performance characteristics 19 Resolution 19 Scan time 19  Installation conditions 20

1
1
1
1
1
1
2
2
2
2
2
2
3
3
5
5
J
6
6
6
6
7
7
7 8
7
7 8
7 <b>8</b> 8
7 8 8
7 8 8 0 0 3
7 8 8 0 0 3
7 8 8 0 0 3 4
7 8 8 0 0 3

## Function and system design

## Application

The Tank Side Monitor NRF590 is a field device for the integration of tank sensors into tank inventory systems. It is used in tank farms, terminals and refineries.

Especially, it can be used in connection with Micropilot M level radars (for inventory control) and Micropilot S high accuracy level radars (for custody transfer applications).


## Operating principle

The Tank Side Monitor is typically installed at the bottom of the tank and allows to access all connected tank sensors. Typical process values measured by the sensors are:

- level
- temperature (point and/or average)
- water level (measured by capacitive probe)
- hydrostatic pressure (for hydrostatic tank gauging, "HTG", or hybrid tank measurements, "HTMS")
- secondary level value (for critical applications)

The Tank Side Monitor collects the measured values and performs several configurable tank calculations. All measured and calculated values can be displayed at the on-site display. Via a field communication protocol, the Tank Side Monitor can transfer the values to an inventory control system.

# System Integration (typical example)

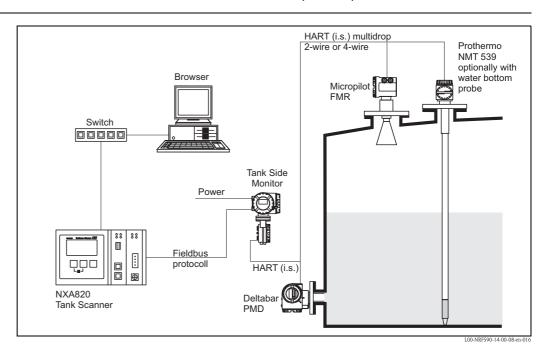

HART interface	
----------------	--

IS (intrinsically safe)	HART Master for measuring device connection			
Non-IS (if selected by order code)	user settable:  HART Master HART Slave (active 4-20 mA when address is "0")			

# Power supply for HART instruments

The Tank Side Monitor provides intrinsically safe power for 2-wire tank sensors. It also can provide intrinsically safe power for the 4-wire instrument Micropilot S.

# Operation of HART instruments

For the following instruments, the operating menu can be accessed on the display of the Tank Side Monitor:

- Micropilot M: FMR230/231/240/244/245
- Micropilot S: FMR530/531/532/533/540
- Prothermo: NMT532/535/536/537/538
- Prothermo: NMT539 (including Water Bottom Probe)
- Cerabar M: PMC/PMP4x
- Cerabar S: PMC/PMP7x
- Cerabar: PCM/PMC73x/63x
- Deltabar: PMD/FMD23x/63x
- Deltabar S: PMD/FMD7x

Any other HART instrument can be operated via the Generic HART menu (allowing all 4 universal HART values to be accessed).

## Typical Tank calculations

Setup preset	Installation example	Sensors	measured/ calculated values	required parameters
Direct level measurem	ent			
Level only	Micropilot Tank Side Monitor  Loo-NRF590-14-00-08-yy-002	■ Level sensor	■ level	■ Tank Ref Height
Level + Temperature	Prothermo Micropilot  Tank Side Monitor  Loo-NRF590-14-00-08-yy-003	■ Level sensor ■ Temperature sensor (RTD or HART device; optionally with bottm water probe)	■ level ■ temperature	
Hybrid Tank Measurin	ng System (HTMS)	T	T	
HTMS + P1	Micropilot  Tank Side Monitor  P1 Position  P1  L00-NRF590-14-00-08-yy-004	<ul><li>Level sensor</li><li>Pressure sensor (P1, bottom)</li></ul>	level     density of the measured medium (calculated)	<ul> <li>Tank Ref Height</li> <li>P1 Position</li> <li>Min HTMS (minimum level at which HTMS measurement is possible; should be slightly above the position of the P1 sensor)</li> <li>local gravity</li> <li>vapour density</li> <li>air density</li> <li>P3 Position (only for the "HTMS + P1,3" mode)</li> </ul>
HTMS + P1,3  Note! This mode should be used in non-atmospheric tanks (e.g. pressurised tanks)	Tank Side Monitor  P1  L00-NRF590-14-00-08-yy-005	<ul> <li>Level sensor</li> <li>Pressure sensor (P1, bottom)</li> <li>Pressure sensor (P3, top)</li> </ul>		

Setup preset	Installation example	Sensors	measured/ calculated values	required parameters		
Hydrostatic Tank Gaug	ging (HTG)		l			
HTG P1	Tank Side Monitor  P1 Position → P1  L00-NRF590-14-00-08-yy-006	■ Pressure sensor (P1, bottom)	■ level (calculated)	<ul> <li>Tank Ref Height</li> <li>local gravity</li> <li>density of the measured medium</li> <li>Min HTG Level         (minimum level at which HTG         measurement is possible; should be         slightly above the position of the P1         sensor)</li> <li>P1 Position</li> <li>P3 Position (only for the "HTG P1,3"         mode)</li> </ul>		
HTG P1,3  Note! This mode should be used in non-atmospheric tanks (e.g. pressurised tanks)	Tank Side Monitor  P1 Position P1  L00-NRF590-14-00-08-yy-009	<ul> <li>Pressure sensor</li> <li>(P1, bottom)</li> <li>Pressure sensor</li> <li>(P3, top)</li> </ul>		mode)		
HTG P1,2	Tank Side Monitor P1-P2 Distance P1 Position P1 P0-P1 DO-NRF590-14-00-08-yy-007	<ul> <li>Pressure sensor (P1, bottom)</li> <li>Pressure sensor (P2, middle)</li> </ul>	level (calculated)     density of the measured medium (calculated)	<ul> <li>Tank Ref Height</li> <li>local gravity</li> <li>Min HTG Level (minimum level at which HTG measurement is possible; should be slightly above the position of the P2 sensor)</li> <li>P1 Position</li> <li>P1-P2-Distance</li> <li>P3 Position (only for the "HTG</li> </ul>		
HTG P1,2,3  Note! This mode should be used in non-atmospheric tanks (e.g. pressurised tanks)	P1-P2 Distance P1 P1 Position P1 L00-NRF590-14-00-08-yy-008	■ Pressure sensor (P1, bottom) ■ Pressure sensor (P2, middle) ■ Pressure sensor (P3, top)		P1,2,3" mode)		

### Corrections

The Tank Side Monitor can automatically calculate the following corrections:

- Correction for the Hydrostatic Tank Deformation (HyTD)
- Temperature Correction for Thermal Expansion of the Tank Shell (CTSh)

## Overfill protection

The NRF590 can be configured and used as part of an overfill protection system in comjunction with the approved WHG operating mode of the Endress+Hauser FMR53x/54x radar devices (as described in the TÜV test certificate for the FMR53x/54x WHG operating mode).

## Overview


- Level input from FMR53x/54x via HART communication
- Discrete output via DO #A and/or DO #B (in conjunction with the AL1 alarm function block
- Analogue 4 to 20mA output via AO



### Note!

AO #2 and DO #C (if available) cannot be used for overfill protection

## Inputs and outputs

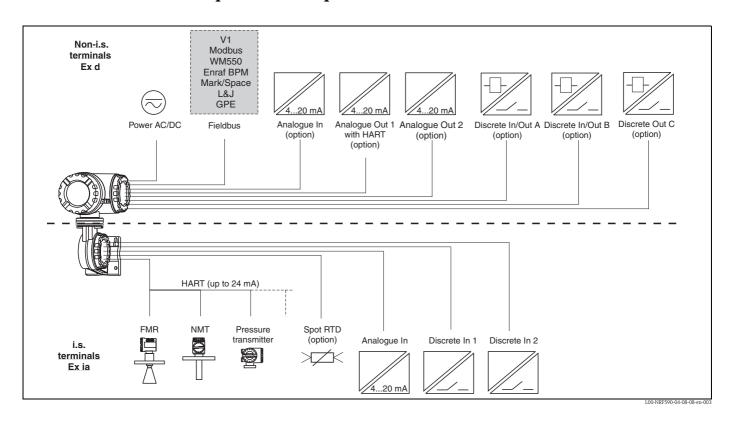

## Non IS inputs and outputs

		V1	Modbus	WM550	ВРМ	Mark/ Space	L&J Tankway	GPE
Analogue In	AI	-	option <sup>1)</sup>	-	standard	standard	standard	-
Analogue Out 1	AO	standard +HART	option¹ +HART	standard +HART	standard +HART	standard +HART	standard +HART	standard +HART
Analogue Out 2	AO#2	standard	-	standard	-	-	-	standard
Discrete In/Out A	DI#A DO#A	option, s. pos. 50 of the product structure						
Discrete In/Out B	DI#B DO#B	option, s. pos. 60 of the product structure						
Discrete Out C	DO#C	standard	-	-	-	_	-	-

1) see pos. 20 option 4 of the product structure; Modbus without in- or output does **not** provide an Ex d HART bus!

## IS inputs and outputs

	V1 Modbus WM550 BPM Mark/Spac		Mark/Space	L&J Tankway	GPE			
HART	HART		standard	standard	standard	standard	standard	standard
IS RTD			option, s. pos. 40 of the product structure					
IS Discrete In 1	IS DI#1	standard	standard	standard	standard	standard	standard	standard
IS Discrete In 2	IS DI#2	standard	standard	standard	standard	standard	standard	standard
IS Analogue In	IS AI	standard	standard	standard	standard	standard	standard	standard

#### Fieldbus Protocols

The Tank Side Monitor NRF590 supports all of the following industry standard communication protocols allowing it to be integrated with existing instrumentation and connect to host computer systems without the need for additional hardware. These protocols allow for piece-by-piece replacement and upgrading of older technologies to modern radar solutions.

#### Sakura V1

V1 protocol provides a standard form of digital communication via a two-wire system. V1 was brought to the market by Sakura Endress and meets the demands of the Japanese market.

The Tank Side Monitor implementation of the V1 slave protocol supports various old and new V1 protocols:

- V1 (new V1)
- MDP (old V1)
- BBB (old V1)
- MIC+232 (old V1) (in preparation)

### EIA-485 (RS485) Modbus

In Modbus, the flow of data between two devices uses a master/slave protocol. The NRF590 acts as a Modbus slave and runs on the EIA-485 (RS) version of the MODBUS communications board. Modbus provides Varec MFT parameter mapping for easier setup in retrofit applications. It provides direct connection to PLC and DCS systems.

#### Whessoematic WM550

The WM550 protocol provides a standard form of digital communication via dual current loops. WM550 was developed by Endress+Hauser (formerly Whessoe) to facilitate communications to transmitters installed on mechanical float and tape gauges. It is a two-wire system and the only protocol with a redundant loop.

#### **BPM**

The Bi-Phase Mark (BPM) protocol provides compatibility to Enraf systems by emulating the Enraf GPU-BPM protocol. The NRF590 is fully compatible to ENRAF (802, 812), 811, 854 and 954 series servo gauges, 813 MGT (mechanical gauge transmitter), 872, 873 and 973 series Radar gauges, 874 AIM (Analogue Input Module) and the 875 VCU (Valve Command Unit).

## Mark/Space

The Mark/Space protocol provides compatibility with Varec transmitters using a standard form of digital communication via a voltage mode bus. Mark/Space was developed to facilitate communication to transmitters installed on mechanical float and tape gauges. It supports product level, temperature and discrete inputs.

## L&J Tankway

L&J Tankway protocol provides a standard form of digital communication via a voltage mode bus. Tankway supports product level, temperature and discrete inputs.

## **GPE**

GPE protocol provides a standard form of digital communication via a current loop. It is compatible with L&J and GPE mechanical float and tape and servo instrumentation.

## Values transmitted by the Field Protocols

The following values can be transmitted by the communication protocols:

Tank Value	Symbol	V1 - old	V1 - new	Modbus	WM550	ВРМ	Mark/ Space	L&J Tankway Basic	L&J Tankway Servo	GPE
Level	L	yes	yes	yes	yes	yes	yes	yes	yes	yes
Temperature (Product)	T <sub>P</sub>	yes	yes	yes	yes	yes	yes	yes	yes	yes
Observed Density	D <sub>obs</sub>	-	yes	yes	yes	yes	-	-	yes	-
Water Level	L <sub>W</sub>	-	yes	yes	yes	yes	-	-	yes	-
Pressure 1 (Bottom)	P <sub>1</sub>	-	yes	yes	yes <sup>1</sup>	yes	-	-	-	-
Pressure 2 (Middle)	$P_2$	-	yes	yes	yes <sup>1)</sup>	-	-	-	-	-
Pressure 3 (Top)	$P_3$	-	yes	yes	yes	yes	-	-	-	-
Measured Level	L <sub>M</sub>	-	-	yes	yes1	-	-	-	-	-
Level Correction	L <sub>C</sub>	-	-	yes	yes <sup>1</sup>	-	-	-	-	-
Percentage Level	L <sub>%</sub>	-	-	yes	yes	-	-	-	-	-
Gasphase Temperature	T <sub>V</sub>	-	yes	yes	yes1	yes	-	-	-	-
Air Temperature	T <sub>A</sub>	-	-	yes	yes <sup>1</sup>	yes	-	-	-	-
Level Flow Rate (Rate of change of level)		-	-	yes	yes <sup>1</sup>	-	-	_	-	-
Volumetric Flow Rate		-	-	yes	yes <sup>1</sup>	-	-	-	-	-
General Purpose Value 1	GP <sub>1</sub>	-	yes	yes	yes1	-	-	-	-	-
General Purpose Value 2	GP <sub>2</sub>	-	yes	yes	yes1	-	-	-	-	-
General Purpose Value 3	GP <sub>3</sub>	-	-	yes	yes1	-	-	-	-	-
General Purpose Value 4	GP <sub>4</sub>	-	-	yes	yes1	-	-	-	-	-
Multi-Element Temperatures	T <sub>(1)</sub> to T <sub>(16)</sub>	-	yes	yes	T <sub>(1)</sub> to T <sub>(15)</sub>	-	-	-	-	-
Alarm/Discrete Values		yes <sup>2)</sup>	yes <sup>2</sup>	yes	yes	yes <sup>3)</sup>	yes <sup>4)</sup>	yes <sup>5)</sup>	yes <sup>5</sup>	-
Discrete Output Control		-	-	yes	-	-	-	-	-	1
Additional		-	4-20mA <sup>6)</sup>	yes	Level %	-	-	Temp <sup>7)</sup>	-	4-20mA <sup>6</sup>
Protocol Documentation		KA00246F	KA00246F	KA00245F	KA00247F	KA00248F	KA00249F	KA00250F	KA00250F	KA00251F

- Only accessible through WM550 extended tasks (51&52); not available on older control room systems.
- $\ \ \, \hbox{The protocol allows 2 alarm and 4 general purpose flags which can be connected to any alarm or discrete input.}$
- 3) Level L & H alarm, 4 alarms and 2 general purpose flags which can be connected to any alarm or discrete input.
- 4) The protocol allows 2 digital alarm values which can be connected to any alarm or discrete input.
- 5) The protocol allows 2 digital values which can be connected to any alarm or discrete input.
- 6) One additional value "4-20mA" which can be connected to any value, however range of value sent is limited (see KA00246F/00/EN).
- 7) One additional value "Temp2" which can be connected to any value, however the range of value sent is limited (see KA00250F/00/EN).

# Technical data of the non-IS inputs and outputs

## Analogue 4 to 20 mA input (option, s. pos. 20 of the product structure)

Internal load (to ground)	110 Ω
Measuring range	0 to 26 mA
Accuracy	$\pm 15~\mu A$ (after linearisation and calibration)

## Analogue 4 to 20 mA outputs

Output current	3 to 24 mA
Output voltage	$U = 24 \text{ V} - I_{LOAD} \text{ 400 } \Omega$
Output load	max. 500 $\Omega$
Accuracy	$\pm 15~\mu A$ (after linearisation and calibration)
HART options <sup>1)</sup>	<ul> <li>Slave, address # 0:         4 to 20 mA active</li> <li>Slave, address #1 - #15:         fixed current (user selectable)</li> <li>Master:         max. current (≤ 24 mA) selectable by user;         typically 6 HART instruments (each 4 mA) can be connected<sup>2)</sup></li> </ul>

- 1) The second analogue output (available for V1, WM550 and GPE) has no HART option.
- 2) Start-up current of the HART instruments has to be taken into account

## Discrete inputs/outputs A and B

The Tank Side Monitor can be equipped with 1 or 2 discrete I/O modules. Available types: see position 50 and 60 of Product Structure or chapter "Accessories".

## Discrete output C (for V1 protocol)

Load voltage	3 to 100 V
Load current	max. 500 mA
Type of contact	mechanical latching relay
Isolation voltage	1500 V
Approvals	UL, CSA

# Technical Data of the IS inputs and outputs

## HART input loop

Source voltage	$U = 25 \text{ V} - I_{Load} \text{ x } 333 \Omega \text{ (typically)}$	
total I <sub>max</sub>	Start-up currents of all connected HART devices may not exceed a total of 27 mA	
connectable sensors	depending on current consumption (including start-up current)	

## Spot RTD input (option, s. pos. 40 of the product structure)

Measuring range	10600 Ω
Excitation current	typ. 400 μA, max. 2000 μA

Type of Sensor	Nominal value	Temp <sub>min</sub>	Temp <sub>max</sub>	Accuracy <sup>1)</sup>
Pt100 (385) IEC751 Pt100 (389) Pt100 (392) IPTS-68	100 Ω @ 0 °C (≈ 32 °F)	-200 °C (≈ -330 °F)	+600 °C (≈ +1110 °F)	±0.1 °C (≈ ± 0.2 °F)
Cu90 (4274)	100 Ω @ 25 °C (≈ 77 °F) [90 Ω @ 0 °C (≈ 32 °F)]	-100 °C (≈ -150 °F)	+250 °C (≈ +480 °F)	±0.1 °C (≈ ± 0.2 °F)
Ni120 (672)	120 Ω @ 0 °C (≈ 32 °F)	-60 °C (≈ -75 °F)	+180 °C (≈ +350 °F)	±0.1 °C (≈ ± 0.2 °F)
Ni100 (618) DIN 43760	100 Ω @ 0 °C (≈ 32 °F)	-60 °C (≈ -75 °F)	+180 °C (≈ +350 °F)	±0.1 °C (≈ ± 0.2 °F)

<sup>1)</sup> Accuracy of converter, may be influenced by element accuracy

## IS Analogue 4 to 20 mA input (option, s. pos. 70 of the product structure)

Source voltage	$U = 25 \text{ V} - I_{\text{Load}} \times 333 \Omega \text{ (typically)}$
Internal load (to ground)	100 Ω
Measuring range	0 to 26 mA
Accuracy	$\pm 15~\mu A$ (after linearisation and calibration)
Usage	Source for Discrete Inputs / Source for 4 to 20 mA loop device

## Discrete inputs (option, s. pos. 70 of the product structure)

Active voltage ("closed circuit")	min. 9 V (default)
In-active voltage ("open circuit")	max. 7 V (default)
Active high current	4 mA
Switching hysteresis	2 V


12

## Auxiliary energy

AC supply	55 to 264 VAC; insensitive to polarity $/$ CSA approved: 55 to 250 VAC
DC supply	18 to 55 VAC/DC
Power consumption	<ul> <li>370 mA at 24 V DC</li> <li>200 mA at 48 V DC</li> <li>75 mA at 125 V AC</li> <li>45 mA at 220 V AC</li> </ul>
Fuse	Internal (on primary power)

## Grounding


The NRF590 must be grounded to the tank potential before communication and power connections are made. The connections (A  $\geq$  4mm²) from each outer ground plug of the NRF590 to the tank ground must be made before any other wiring connections are made. All grounding must be compliant with local and company regulations and checked before the equipment is commissioned.

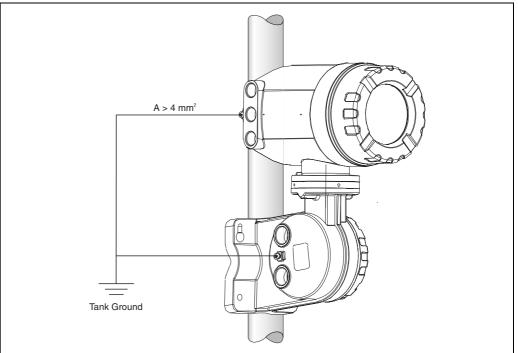

L00-NRF590-04-08-08-en-00

## Electrical connection - non-i.s. terminals

# Terminal assignment of the field protocol/host side

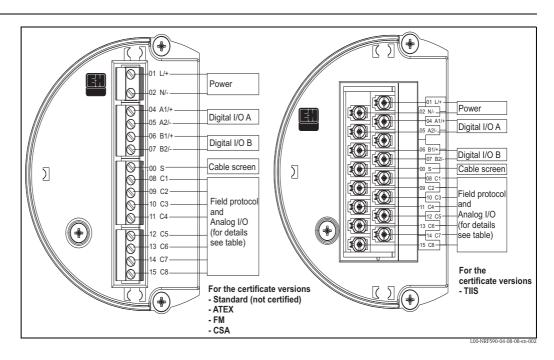

Terminal	01	02	04	05	06	07	00
	L/+	N/-	A1/+	A2/-	B1/+	B2/-	S
	Power	supply	Discrete I/O - A +	Discrete I/O - A -	Discrete I/O - B +	Discrete I/O - B	Cable screen

	08 C1	09 C2	10 C3	11 C4	12 C5	13 C6	14 C7	15 C8
V1	4 to 20 mA output <sup>1)</sup> #2	V1A	V1B	0 V <sup>1</sup>	0 V	4 to 20 mA output #1 + HART	discrete output 1C	discrete output 2C
EIA-485 Modbus	not used <sup>2)</sup>	485-B	485-A	0 V	0 V <sup>1</sup>	4 to 20 mA output <sup>3)</sup> +HART	4 to 20 mA input <sup>3</sup>	+24 V¹
Whessoe WM550	4 to 20 mA output <sup>1</sup> #2	Loop 1-	Loop 1+	0 V <sup>1</sup>	0 V	4 to 20 mA output #1 +HART	Loop 2-	Loop 2+
ВРМ	not used <sup>2</sup>	Т	Т	0 V	0 V <sup>1</sup>	4 to 20 mA output + HART	4 to 20 mA input	+24 V¹
Mark/Space	V+	Space	Mark	0 V (V-)	0 V <sup>1</sup>	4 to 20 mA output + HART	4 to 20 mA input	+24 V¹
L&J Tankway	Power	Encoder	Computer	Ground	0 V <sup>1</sup>	4 to 20 mA output + HART	4 to 20 mA input	+24 V¹
GPE	4 to 20 mA output <sup>1</sup> #2	Loop 1-	Loop 1+	0 V <sup>1</sup>	0 V	4 to 20 mA output #1 + HART	do not connect	do not connect

- 1) In case an "Ex d" rated 4-wire level gauge version is used, the power supply can be obtained from these terminals (21V  $\pm$ 10%).
- 2) The internal voltage at this terminal is 0 V, however, shielding and signal common should be connected to terminal 11 or 12.
- 3) Option, s. pos. 20 of the product structure

## Connection of the field protocols

#### Sakura V1

The V1 protocol provides 2 wire communication allowing up to 10 devices to operate on a loop. V1 connects to terminals 9-10. Max. distance: 6000 m

#### EIA-485 Modbus

The NRF590 protocol uses a shielded 3-wire EIA-485 hardware interface to communicate with the modbus master. EIA-485 is a high speed, differential communications network that allows up to 32 devices to operate on one network.

- Using one shielded twisted pair of 18 AWG wire, connect the EIA-485 at terminal 9 and 10.
- Termination of the EIA-485 bus at the NRF590 can be set in the operating menu (only enable on end device in a loop)
- Connect the 3rd wire from the control system signal common (0V) to terminal 11 or 12.
- Max distance: 4000 ft (1300 m)

### Whessoematic WM550

The WM550 protocol provides 2 wire, current loop communication and allows up to 16 devices per loop. For redundancy (safety function) two wire pairs are used. They always transmit the same values. The WM550-loops connect to terminals 9 - 10 and 14 - 15. Max. distance: 7000 m

#### **BPM**

The BPM protocol provides 2 wire communication allowing up to 10 devices to operate on a loop. BPM connects to terminals 9-10. Max. distance:  $10000\,\mathrm{m}$ 

### Mark/Space

For a NRF590 using the Mark/Space field communications option, the following additional wiring connections must be made:

- Run 2 twisted pairs (one power, one communication) of 18 AWG wire (Mark/Space wires) into the upper terminal compartment through one of the conduit entries along with the 48 Vdc power wiring.
- Connect the Mark line to terminal 10 and the Space line to terminal 9.
- Connect to power supply at terminals 8 and 11.

## L&J Tankway

Including power and ground, L&J is a 4-wire system, allowing 50+ devices to be connected on the communication bus. L&J connects to terminals 8 through 11.

#### **GPE**

The GPE protocol provides 2 wire current loop communication. GPE connects to terminal 9-10.

## Grounding of the fieldbus screen


The screen of the fieldbus cable should be connected to ground at both ends. If this is not possible due to signal disruption by potential equalisation currents, it is advisable to connect the screen of the fieldbus cable to terminal "00 S" at the NRF590 and to ground at the other end. The "00S" terminal provides a 500 V capacitor between the cable screen and tank ground potential.

# Connection of the auxiliary energy

The Tank Side Monitor can be AC or DC supplied, depending on the installed power supply board. The AC supply needs to be connected to the terminals marked "L/+" (Line) and "N/-" (Neutral), corresponding with the phase/line and neutral wire. DC supply can be connected to the same terminals, for which it is necessary to connect the positive (+) to the terminal marked "L/+", and the negative to the terminal marked "N/-".

# Connection of the non-i.s. 4 to 20 mA analogue input

Depending on the selected fieldbus communication board, a non-i.s. self-powered or loop powered analogue transmitter can be connected. The analogue signal for the loop powered transmitter can be connected to the terminals 14 (-) and 15 (+24 V DC). The maximum supply current for the analogue transmitter is limited to 24 mA. The analog signal for a self powered transmitter should be connected to terminals 11 or 12 and 14.




Connection of the non-i.s. 4 to 20 mA analogue output

For all field communication boards except the Modbus Option without analog in/output, a non-i.s. 4.. .20mA output is available. Via Software settings, this analogue output can be connected to any parameter in the Tank Side Monitor. The analogue output is available between terminals 13 (+) and 12 (-). From SW 02.01.xx onwards, an additional HART signal is available at terminal 13.

## Connection of the discrete in and output

The Tank Side Monitor can be equipped with up to 2 discrete I/O modules. These modules can be used for interfacing to non-i.s. discrete in- or outputs. Input and output voltage and current ranges depend on the type of selected module installed in the relevant I/O slot. Terminals 4 and 5 correspond to discrete I/O slot A, terminals 6 and 7 correspond to discrete I/O slot B. For details on available I/O modules,  $\rightarrow \stackrel{\triangle}{=} 30$ .

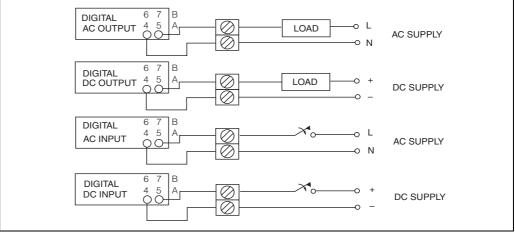

L00-NRF590-04-00-08-en-004


Note!

 $250\ V\ AC$  is the maximum load that can be connected.

16

## Electrical connection - i.s. terminals

## Terminal assignment

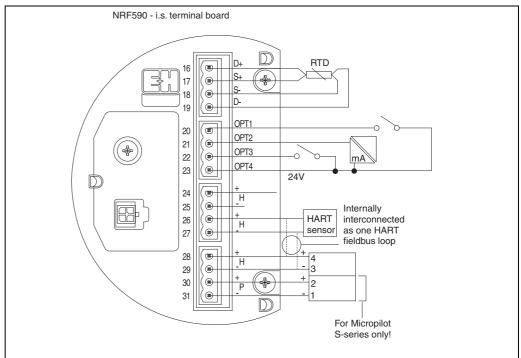

L00-NRF590-04-00-08-en-018

Terminal	Designation	Meaning	
16	D+	+ RTD drive <sup>1)</sup>	
17	S+	+ RTD sense <sup>1)</sup>	
18	S-	- RTD sense <sup>1), 2)</sup>	
19	D-	- RTD drive <sup>1], 2)</sup>	
20	OPT1	Discrete Input 1	
21	OPT2	Analog Input 1 (4 to 20 mA)	
22	OPT3	Discrete Input 2	
23	OPT4	Option +24 V	
24	H+	+HART comm. <sup>3)</sup>	
25	H-	-HART comm. <sup>4)</sup>	
26	H+	+HART comm. <sup>3)</sup>	
27	H-	-HART comm. <sup>4)</sup>	
28	H+	+HART comm. <sup>3)</sup>	
29	H-	-HART comm. <sup>4)</sup>	
30	P+	+ i.s. power for FMR S-series (terminal 2 of FMR) <sup>3)</sup>	
31	P-	– i.s. power for FMR S-series (terminal 1 of FMR) $^{4)}$	

- 1) These terminals should be left unconnected if RTD has not been selected in feature 40 of the product structure.
- 2) For a 3-wire RTD, terminals 18 and 19 should be connected together.
- 3) These terminals share the same HART signal.
- 4) These terminals share the same i.s. 0 V signal.

## Connection of HART instruments

#### Tank sensors


The Tank Side Monitor can interface to a maximum of 6 i.s. HART sensors. All HART sensors are connected to one HART multi-drop communication loop. In order to keep wiring simple, 3 interconnected terminal pairs are available. The terminal pairs are marked respectively "H+" and "H-".

## Power supply for Micropilot S


For supplying extra i.s. power to the FMR S-series radar, additional power terminals are available, marked as "P+" and "P-". Although it is possible to use only 3 wires between the S-series radar and the NRF590, by combining the "P-" and "H-" wires, it is recommended to use a double pair of screened and twisted cable.

### Grounding of the cable screen (for Micropilot S)

The screen of the cable connecting the Micropilot S to the Tank Side Monitor should be grounded at the Tank Side Monitor,  $\mathbf{not}$  at the Micropilot S.

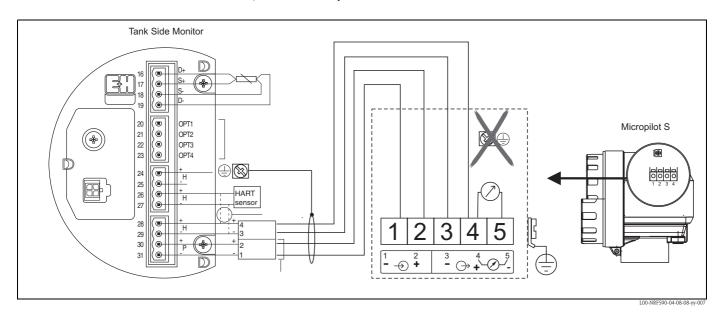

Spot RTD



A spot RTD can be connected to the NRF590 if the option is installed. For 4-wire connection, the RTD must be connected to the 4 available terminals marked D+, S+, S- and D-. For 3-wire connection, the RTD should be connected to the same 4 terminals. The terminals D- and S- should be connected together directly at the NRF590 terminals.

18

## Performance characteristics

### Accuracy

#### **HART** sensors

Accuracy of all data from connected HART sensors depends on the type and installation of instruments. The use of the digital HART protocol prevents accuracy data degradation, as would be the case with analogue (4 to 20 mA) sensors.

### Spot RTD input, analogue inputs, analogue outputs

See "Technical data of the IS inputs and outputs".

### Resolution

Resolution of all measured data depends on sensor and communication settings. The following settings are recommended for inventory and custody transfer applications:

Data type	Units	Inventory control	Custody transfer
	millimeters	1 mm	1 or 0.1 mm
	meters	10 mm	1 or 0.1 mm
Level	feet	0.01 ft	0.01 ft
	inches	1" or 0.1"	0.01" or 0.001"
	ft-in-16	1/16"	1/16"
Toronoroturo	°C	0.1 °C	0.1 °C
Temperature	°F	0.1 °F	0.1 °F

For purpose of consistency all internal calculations are performed in SI units.

### Scan time

### **HART** sensors


The data of connected HART sensors is constantly scanned and updated in the internal data base. The scanning sequence is based on the priorities of the measurements (level – prio 1, temperature – prio 2, pressure – prio 3,...). Typically, a value change on the HART multidrop loop is displayed after a 2 seconds delay (for priority 1 values).

## Spot RTD input


RTD resistance is measured and recalculated at least every second.

## Installation conditions


## Wall mounting

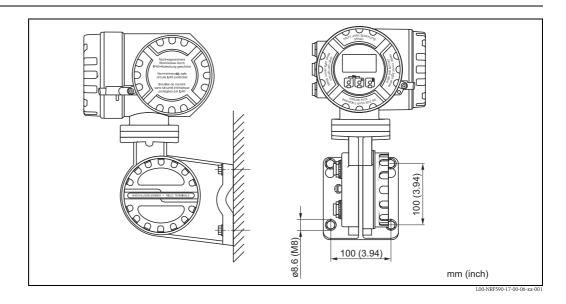

## Mounting on vertical rail

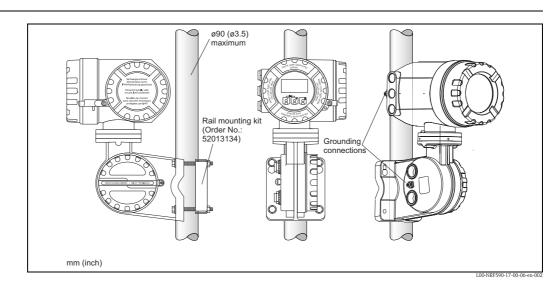

## Mounting on horizontal rail

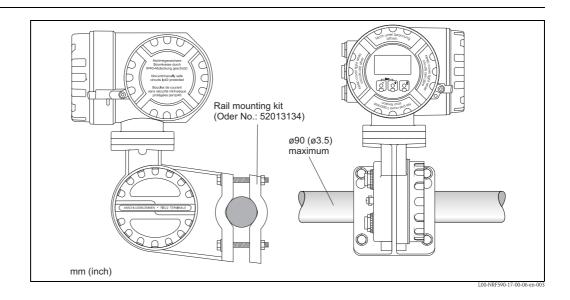


## **Ambient conditions**

Ambient temperature	-40 °C to +60 °C (-40 °F to +140 °F)
Storage temperature	-55 °C to +85 °C (-67 °F to +185 °F)
Ingress protection	IP65, Nema 4X
Electromagnetic compatibility (EMC)	■ Interference emission to EN 61326, Equipment class A ■ Interference immunity to EN 61326 Use shielded signal lines for installation.
Overvoltage protection	Both interfaces of the NRF590 - the Ex ia and the Ex d side - are protected by internal 600 Vrms surge arresters which have been tested against 10 kA transient discharges.

## Mechanical construction

### Design, dimensions

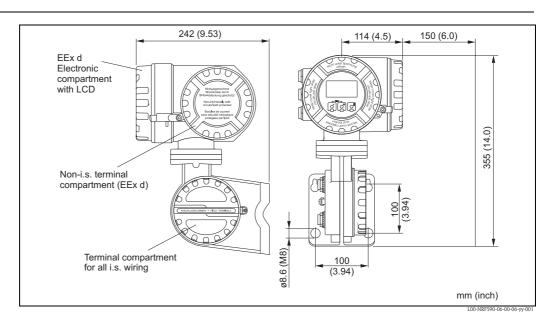

Material

- Remote field housing: powder coated die-cast aluminium
- Wall-mount housing: powder coated die-cast aluminium
- Window material: glass

#### Construction

The NRF590 housing has three separate compartments, one containing all electronics and two for electrical connections. The enclosure is die-cast aluminum with an polyester coating and IP65 (NEMA 4) rating. The upper terminal compartment and electronics compartment are designated for non-i.s. connections and electronics and are rated EEx d.The lower terminal compartment is designated for i.s. wiring connections and wiring only.

### Weight

## approx. 8 kg

### Cable entries

The non-i.s. terminal compartment has 3 cable entries. The threading in this terminal compartment enclosure is M20x1.5. All intrinsically designated wiring has to be terminated in the i.s. terminal compartment. For the i.s. wiring, two M25x1.5 cable entries are available. The internal diameter of the cable entry is 16 mm. For accommodating various types of cable glands or cable conduit (rigid or flexible), the following sizes of cable gland adapters are optionally available:

- M20x1.5
- G½
- 1/2" NPT
- 3/4" NPT (max. 2 cable entries)

All adapters are rated EEx d and can be used for either cable connection. When installing, properly seal all ports to prevent moisture or other contamination from entering the wiring compartments.

22

## Human interface


# Display and operating elements

## Liquid crystal display (LCD)

Four lines with 20 characters each. Display contrast adjustable through key combination.

The backlight of the display is activated during operation for user defined time (30 sec continuous backlight). The following display languages can be selected by the user:


- English
- German
- Japanese<sup>1)</sup>
- Simplified Chinese<sup>2)</sup>
- Dutch
- Spanish
- French
- Italian

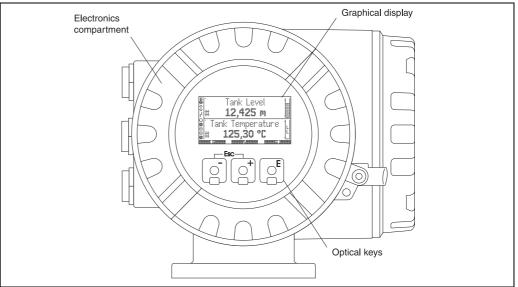

L00-NRF590-07-00-00-en-001

## Optical keys

The optical keys allow the Tank Side Monitor to be operated without the housing being opened. From Software Version 02.xx.xx onwards they function as softkeys, i.e. their meaning varies depending on the current position within the operating menu. The meaning is indicated by softkey symbols in the bottom line of the display:

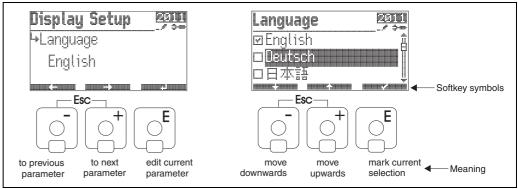

L00-NRF590-07-00-00-en-00

<sup>1)</sup> Japanese font: JIS X 208-1997 including Hiragana, Katakana asnd Kanji

<sup>2)</sup> Chinese font: GB18030, CITS Committee approved

## Format of decimal numbers


The number of decimal places displayed can be selected from three resolution presets (high, normal, low)

VAlue		resolution pres	et
	low	normal	high
level units			
mm	XXXXX	xxxxx	XXXXX.X
cm	XXXX.X	XXXX.X	XXXX.X
m	XX.XXX	xx.xxx	XX.XXXX
in	XXXX.X	xxxxx	XXXX.XX
ft	xxx.xxx	xxx.xxx	xxx.xxx
ft-in-8	xx'xx"x/8	xx'xx"x/8	xx'xx"x/8
ft-in-16	xx'xx"xx/16	xx'xx"xx/16	xx'xx"xx/16
16ths	xxxxx	xxxxx	XXXXX.X
temperature units			
°C	XXX	XXX.X	XXX.XX
°F	XXX	xxx.x	XXX.XX
pressure units			
Pa	xxxxxx	xxxxxx	XXXXXX
kPa	xxxx.x	xxxx.xx	XXX.XXX
MPa	x.xxxx	x.xxxx	x.xxxxx
mbar	xxxxx	xxxxx	XXXXX.X
bar	xx.xxx	xx.xxx	XX.XXXX
psi	XXX	XXX.X	XXX.XX
inH <sub>2</sub> 0	xxxxx	xxxxx.x	XXXXX.X
density units	,	,	,
kg/m <sup>3</sup>	xxxx.x	xxxxxx	xxxx.xx
g/ml	x.xxxx	x.xxxx	x.xxxx
lb/ft <sup>3</sup>	xx.xx	xx.xxx	xx.xxx
°API	xxx.xx	xxx.xx	XXX.XXX
current units	1	1	
mA	XX.XXX	XX.XXX	XX.XXXX

## Operating concept

The Tank Side Monitor is operated via a four-layer menu. The structure of the menu accounts for typical measuring tasks as well as for the individual instrument configuration and installation. In particular, the menu contains dynamic function groups which are only indicated if the respective option is installed or the respective instrument is connected. This structure ensures clarity and simple operation without restricting the scope of functionality.

The appearance and meaning of the LCD change according to the current position within the menu.

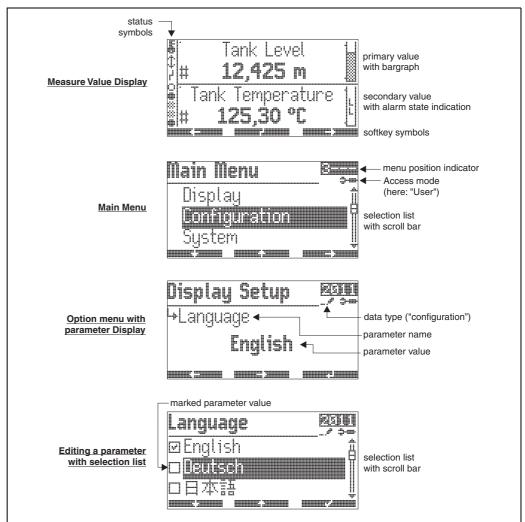

L00-NRF590-07-00-00-en-004

### Remote operation

FieldCare is an Endress+Hauser asset management tool based on FDT technology. With FieldCare, you can configure all Endress+Hauser devices as well as devices from other manufacturers that support the FDT standard. Hardware and software requirements you can find on the internet:

www.endress.com  $\rightarrow$  select your country  $\rightarrow$  search: FieldCare  $\rightarrow$  FieldCare  $\rightarrow$  Technical Data.

FieldCare supports the following functions

- Configuration of transmitter in online operation
- Loading and saving of instrument data (Upload/Download)
- Documentation of measuring point

Certificates	and A	approvals
--------------	-------	-----------

CE mark	The measuring system meets the legal requirements of the EC-guidelines. Endress+Hauser confirms the instrument passing the required tests by attaching the CE-mark.									
Ex approvals	FM									
	FM XP - Class I, Div 1 Groups A-D; Note the Installation Drawings ZD00084F/00/EN and ZD00085F/00/EN (IS 4-20 mA Option Module)									
	CSA									
	FM XP - Class I, Div 1 Groups A-D; Note the Installation Drawings ZD00103F/00/EN and ZD00104F/00/EN (IS 4-20 mA Option Module)									
	ATEX									
	ATEX II 2 (1) G EEx d (ia) IIC T4; Note the Safety Instructions XA00160F/00/A3 and XA00169F/00/A3 (IS 4-20 mA Option Module)									
Custody transfer approvals	<ul><li>NMi type approval</li><li>PTB type approval</li></ul>									

## External standards and guidelines

#### EN 60529

Protection class of housing (IP-code).

#### EN 61010

Safety regulations for electrical devices for measurement, control, regulation and laboratory use.

#### EN 61326

Emissions (equipment class B), compatibility (appendix A - industrial use).

### API MPMS Ch. 3.1A

Standard Practice for Manual Gauging of Petroleum and Petroleum Products in Stationary Tanks.

#### API MPMS Ch. 3.1B

Standard Practice for Level Measurement of Liquid Hydrocarbons in Stationary Tanks by Automatic Tank Gauging.

#### API MPMS Ch. 3.3

Standard Practice fro Level Measurement of liquid Hydrocarbons in Stationary Pressurized Storage Tanks by Automatic Tank Gauging.

#### API MPMS Ch. 3.6

Measurement of Liquid Hydrocarbons by Hybrid Tank Measurement Systems.

### API MPMS Ch. 7.4

Static Temperature Determination Using Fixed Automatic Tank Thermometers.

#### ISO 4266 / Part 1

Petroleum and liquid petroleum products – Measurement of level and temperature in storage tanks by automatic methods – Part 1: Measurement of level in atmospheric tanks.

## ISO 4266 / Part 3

Petroleum and liquid petroleum products - Measurement of level and temperature in storage tanks by automatic methods - Part 3: Measurement of level in pressurized storage tanks (non refrigerated).

## ISO 4266 / Part 4

Petroleum and liquid petroleum products - Measurement of level and temperature in storage tanks by automatic methods - Part 4: Measurement of temperature in atmospheric tanks.

## ISO 4266 / Part 6

Petroleum and liquid petroleum products - Measurement of level and temperature in storage tanks by automatic methods - Part 6: Measurement of temperature in pressurized tanks.

#### ISO 15169

Petroleum and liquid petroleum products – Determination of volume, density and mass of the contents of vertical cylindrical tanks by Hybrid Tank Measurement Systems.

## OIML - R85

Organisation Internationale de Métrologie Légale - Automatic level gauges for measuring the level of liquid in fixed storage tanks.

# Ordering information

## Tank Side Monitor NRF590

This overview doas not mark options which are mutually exclusive.


10	Ap	pproval												
	Α	Non-hazardous areas												
	В	NEPSI Ex d (ia) IIC T6 (in preparation)												
	6	ATEX II 2 (1) EEx d (ia) IIC T6												
	U		CSA XP Cl. I, Div 1, Gr. A-D, zone 1, 2											
	S		FM XP Cl. I, Div 1, Gr. A-D, zone 1, 2											
	K		TIIS EEx d (ia) IIC T4											
	Y	Spe	Special version, TSP-No. to be spec.											
20		Field communication protocol												
		E ENRAF BPM, non-IS 4-20mA input, non-IS 4-20mA HART output												
		G GPE, non-IS 4-20mA HART output  WM550 non-IS 4-20mA output. Wheseve protocol with dual communication												
		1 WM550, non-IS 4-20mA output, Whesoe protocol with dual communication 3 Mark / Space non-IS 4-20mA input-output varies mark / space protocol												
		Mark/Space, non-IS 4-20mA input-output, varec mark/space protocol												
		4 Modbus w/o 4-20mA input+output, EIA 485 5 Modbus, non-IS 4-20mA input+output, EIA 485												
		7	, , , , , , , , , , , , , , , , , , , ,											
		8	1 1											
İ		9												
30			Po	wer	sup	ply								
			Α		_	AC/DC								
			В	55-264V AC										
			Y Special version, TSP-No. to be spec.											
40		Spot RTD option												
				0	Not	selected								
				1	1 Instrinsically safe input									
			9 Special version, TSP-No. to be spec.											
50		Digital Module A												
					Α	Not selected								
					В									
					C Input 3-32V DC									
					D	Input 180-264V AC								
					E G	Input 35-60V AC/DC								
					Н	1								
					H Output 3-60V DC J Output 24-140V AC									
					K Output 4-200V DC									
			R Relay 0-100 VDC, 0-120VAC											
I					Y	Special version, TSP-No. to be spec.								
60						Digital Module B								
						A Not selected								
						B Input 90-140V AC								
						C Input 3-32V DC								
						D Input 180-264V AC								
						E Input 35-60V AC/DC								
						G Output 24-250V AC								
						H Output 3-60V DC								
						J Output 24-140V AC								
İ						K Output 4-200V DC R Relay 0-100 VDC, 0-120VAC								
1			R Relay 0-100 VDC, 0-120VAC Y Special version, TSP-No. to be spec.											
70				 		Additional intrinsically safe module								
70						2   Input 4-20mA + 2x input digital								
						9 Special version, TSP-No. to be spec.								
	/ Opecial version, for the opec.													

80					Cal	Cable entry (Non-IS)							
					F	2 x Ex d gland G1/2							
					В	$2 \times Ex d gland M20 (EEx d > thread M20)$							
					С	2 x Ex d thread G1/2							
					D	2 x I	2 x Ex d thread NPT1/2						
					E	2 x I	Ex d t	hrea	ad NI	PT3/4			
					Н	3 x I	3 x Ex d gland M20 (EEx d > thread M20)						
					K	3 x I	Ex d t	hrea	ad G1	1/2			
					L					PT1/2			
					G					PT3/4 (in preparation)			
					Y	Spec	ial ve	ersion	n, TS	P-No. to be spec.			
90						Entry - IS Compartment							
						2	2x gl	and	M25	5, 13-18mm			
						3	9						
						4	2x th	iread	i NP	T1/2			
						5 2s thread NPT3/4							
						9 Special version, TSP-No. to be spec.							
100					Weight + Measure Approval								
						N Not selected							
						A NMi type approval							
						G PTB type approval							
						Y Special version, TSP-No. to be spec.							
110								Ado	ditio	onal Option			
								0	Basi	c version			
								9	Spec	cial version, TSP-No. to be spec.			
995									Ma	rking			
									1	Tagging (TAG), see additional spec.			
		1	1	1			1	- 1					
NRF590 -						Complete product designation							

## **Accessories**

## Discrete I/O modules

## Standard mechanical diagram for all I/O modules

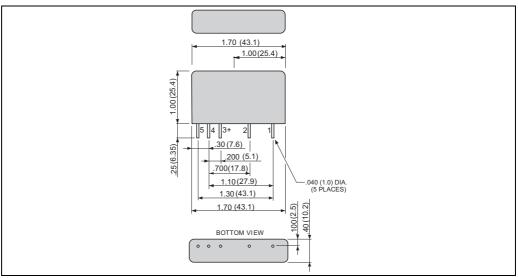


L00-NRF590-00-00-08-en-00

## Output modules

	AC v	oltage	DC voltage			
	VAC  1 2 + 3 WW 4	Zero Voltage Circuit	Vac/oc  Logic  Amplifier  3  WW			
NRF590 order code <sup>1)</sup> module A	NRF590 - ****J*****	NRF590 - ****G*****	NRF590 - ****H*****	NRF590 - ****K*****		
NRF590 order code <sup>1</sup> module B	NRF590 - *****J*****	NRF590 - *****G*****	NRF590 - *****H****	NRF590 - ****K****		
Order Code <sup>2)</sup>	52012959	52012960	52012961	52012962		
Colour of housing	black	black	red	red		
Load voltage	24 to 140 V AC	24 to 250 V AC	3 to 60 V DC	4 to 200 V DC		
Load current	30 to 500	) mA eff. <sup>3)</sup>	20 to 500 mA eff. <sup>1</sup>			
Typ. power dissipation	1 V	V/A	1 to 1.5 W/A			
Transient protection	Meets I	EEE472	Meets IEEE472			
Type of contact		nally open ing turn-on	SPST normally open			
Optical isolation	у	es	yes			
Isolation voltage	4000	V eff.	4000 V eff.			
Approvals	UL, CSA,	CE, TÜV	UL, CSA,	, CE, TÜV		


- 1) This order code is valid if the module is preinstalled in the Tank Side Monitor as module A or module B
- 2) This order code is valid if the module is ordered as an accessory.
- 3) This upper limit of the load current is determined by the Tank Side Monitor.

### Input modules

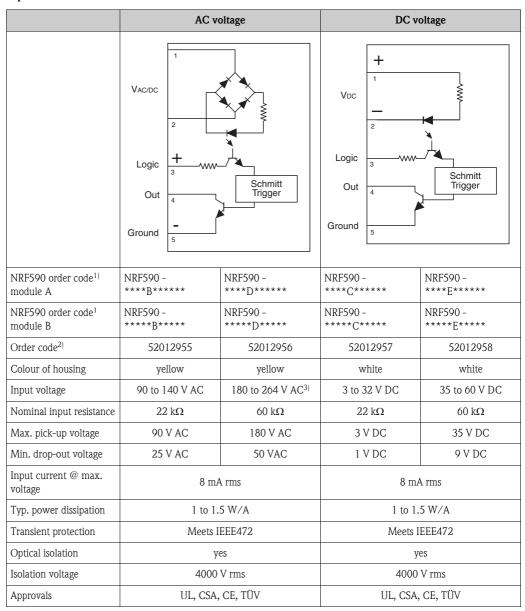

- 1) This order code is valid if the module is preinstalled in the Tank Side Monitor as module A or module B.
- 2) This order code is valid if the module is ordered as an accessory.
- 3) This upper limit of the input voltage is determined by the Tank Side Monitor.


## Relay output module

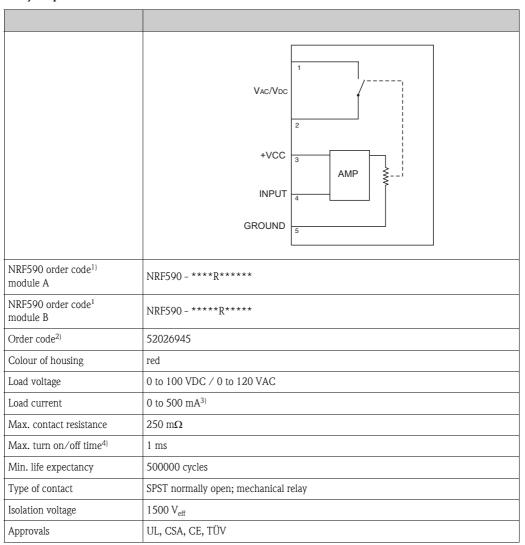

- 1) This order code is valid if the module is preinstalled in the Tank Side Monitor as module A or module B.
- 2) This order code is valid if the module is ordered as an accessory.
- 3) For inductive loads, use diode suppression or RC network to improve contact life.
- 4) Including debounce

## Rail mounting kit

For rail mounting the Tank Side Monitor to vertical or horizontal pipe. Order-Number: 52013134

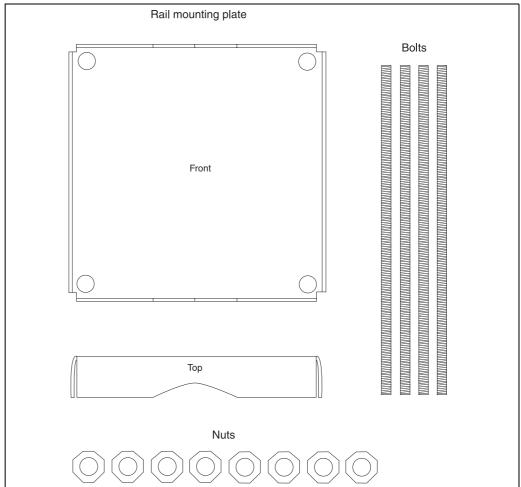

L00-NRF590-00-00-06-en-0

## **Supplementary Documentation**

#### **Technical Information**

### TI00419F/00/EN

Technical Information Tankvision NXA820, NXA821, NXA822

### TI00042N/08/EN

Technical Information Prothermo NMT539

#### TI00216P/00/EN

Technical Information Cerabar S PMC731 / PMP731

#### TI00217P/00/EN

Technical Information Cerabar S PMC631 / PMP635

### TI00344F/00/EN

Technical Information Micropilot S FMR530, FMR531, FMR532, FMR533

#### TI00345F/00/EN

Technical Information Micropilot M FMR230, FMR231, FMR240, FMR244, FMR245

## **Operating Instructions**

### BA00256F/00/EN

Operating Instructions Tank Side Monitor NRF590.

This document describes installation and commissioning of the Tank Side Monitor.

Only those functions of the operating menu are included, which are relevant for a usual application.

### BA00257F/00/EN

Tank Side Monitor - Description of Instrument Functions.

This document contains a detailed description of all the functions of the Tank Side Monitor.

## **Safety Instructions**

## XA00160F/00/A3

Tank Side Monitor NRF590 - ATEX II 2 (1) G

#### XA00169F/00/A3

i.s. 4 to 20mA analogue input module for NRF590 - ATEX II 2 (1) G

## **Control Drawings**

## ZD00084F/00/EN

Tank Side Monitor NRF590 - FM XP - Class I, Div. 1, Groups A-D

#### ZD00085F/00/EN

i.s. 4 to 20mA analogue input module for NRF590 - FM XP - Class I, Div. 1, Groups A-D

## ZD00103F/00/EN

Tank Side Monitor NRF590 - CSA XP - Class I, Div. 1, Groups A-D

#### ZD00104F/00/EN

i.s. 4 to 20mA analogue input module for NRF590 - CSA XP - Class I, Div. 1, Groups A-D

## **Instruments International**

Endress+Hauser Instruments International AG Kaegenstrasse 2 4153 Reinach Switzerland

Tel. +41 61 715 81 00 Fax +41 61 715 25 00 www.endress.com info@ii.endress.com



People for Process Automation

