








# FINESIA 1Piece



Unit: mm

<b>Diameter</b>	Φ3.0 Φ3.2 Φ3.4 Φ3.7 Φ4.2 Φ4.7
<b>Height</b>	7 (S) 9 (M) 11 (L)
<b>Tip Type</b>	 Tapered type (TP) or  Straight type (ST)
<b>Surface Surface Treatment</b>	 HA (HA Coating) or  AO (Anode Oxidization)
<b>Length Intrabony Length</b>	6.0 8.0 10.0 12.0 14.0

## HA Coating

Unit: mm

Diameter		Φ3.4			Φ3.7			Φ4.2			Φ4.7			
Height		S	M	L	S	M	L	S	M	L	S	M	L	
		7	9	11	7	9	11	7	9	11	7	9	11	
<b>Length</b> (Intrabony Length) <b>Tip Type</b>	6.0	TP	-	-	-	-	-	-	-	-	-	-	-	
		ST	-	-	-	●	●	●	●	●	●	●	●	
	8.0	TP	●	●	●	●	●	●	●	●	●	●	●	●
		ST	-	-	-	●	●	●	●	●	●	●	●	●
	10.0	TP	●	●	●	●	●	●	●	●	●	●	●	●
		ST	-	-	-	●	●	●	●	●	●	●	●	●
	12.0	TP	●	●	●	●	●	●	●	●	●	●	●	●
		ST	-	-	-	●	●	●	●	●	●	●	●	●
	14.0	TP	●	●	●	●	●	●	●	●	●	●	●	●
		ST	-	-	-	●	●	●	●	●	●	●	●	●


## Anode Oxidization

Unit: mm

Diameter		Φ3.0			Φ3.2			
Height		S	M	L	S	M	L	
		7	9	11	7	9	11	
<b>Length</b> (Intrabony Length) <b>Tip Type</b>	8.0	TP	●	●	●	●	●	●
		ST	-	-	-	-	-	-
	10.0	TP	●	●	●	●	●	●
		ST	-	-	-	-	-	-
	12.0	TP	●	●	●	●	●	●
		ST	-	-	-	-	-	-
	14.0	TP	●	●	●	●	●	●
		ST	-	-	-	-	-	-

# Implant

HA  
AO  
INSTRUMENTS  
FINESIA 1P

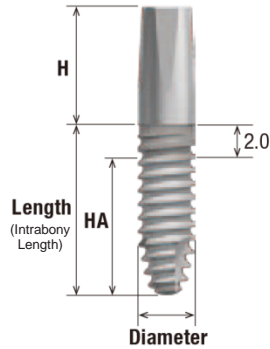

## 1P HA TP

Tapered type


**Diameter  $\phi$  3.4** Unit: mm


Length	HA	H	Product Name	Product Code
8.0	6.0	7.0	F1P-HA-34-8TP-S	BCD014380
		9.0	F1P-HA-34-8TP-M	BCD014381
		11.0	F1P-HA-34-8TP-L	BCD014382
10.0	8.0	7.0	F1P-HA-34-10TP-S	BCD014383
		9.0	F1P-HA-34-10TP-M	BCD014384
		11.0	F1P-HA-34-10TP-L	BCD014385
12.0	10.0	7.0	F1P-HA-34-12TP-S	BCD014386
		9.0	F1P-HA-34-12TP-M	BCD014387
		11.0	F1P-HA-34-12TP-L	BCD014388
14.0	12.0	7.0	F1P-HA-34-14TP-S	BCD014389
		9.0	F1P-HA-34-14TP-M	BCD014390
		11.0	F1P-HA-34-14TP-L	BCD014391

**Diameter  $\phi$  3.7** Unit: mm

Length	HA	H	Product Name	Product Code
8.0	6.0	7.0	F1P-HA-37-8TP-S	BCD014403
		9.0	F1P-HA-37-8TP-M	BCD014404
		11.0	F1P-HA-37-8TP-L	BCD014405
10.0	8.0	7.0	F1P-HA-37-10TP-S	BCD014406
		9.0	F1P-HA-37-10TP-M	BCD014407
		11.0	F1P-HA-37-10TP-L	BCD014408
12.0	10.0	7.0	F1P-HA-37-12TP-S	BCD014409
		9.0	F1P-HA-37-12TP-M	BCD014410
		11.0	F1P-HA-37-12TP-L	BCD014411
14.0	12.0	7.0	F1P-HA-37-14TP-S	BCD014412
		9.0	F1P-HA-37-14TP-M	BCD014413
		11.0	F1P-HA-37-14TP-L	BCD014414

Length = (Intrabony Length)



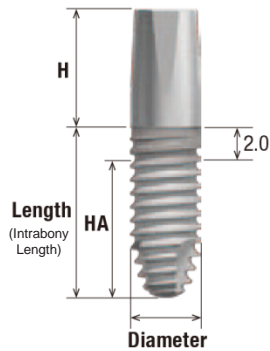

## 1P HA TP

Tapered type

Diameter			$\phi$ 4.2	Unit: mm
----------	--	--	------------	----------

Length	HA	H	Product Name	Product Code
8.0	6.0	7.0	F1P-HA-42-8TP-S	BCD014423
		9.0	F1P-HA-42-8TP-M	BCD014424
		11.0	F1P-HA-42-8TP-L	BCD014425

10.0	8.0	7.0	F1P-HA-42-10TP-S	BCD014426
		9.0	F1P-HA-42-10TP-M	BCD014427
		11.0	F1P-HA-42-10TP-L	BCD014428

12.0	10.0	7.0	F1P-HA-42-12TP-S	BCD014429
		9.0	F1P-HA-42-12TP-M	BCD014430
		11.0	F1P-HA-42-12TP-L	BCD014431

14.0	12.0	7.0	F1P-HA-42-14TP-S	BCD014432
		9.0	F1P-HA-42-14TP-M	BCD014433
		11.0	F1P-HA-42-14TP-L	BCD014434

Diameter			$\phi$ 4.7	Unit: mm
----------	--	--	------------	----------

Length	HA	H	Product Name	Product Code
8.0	6.0	7.0	F1P-HA-47-8TP-S	BCD014443
		9.0	F1P-HA-47-8TP-M	BCD014444
		11.0	F1P-HA-47-8TP-L	BCD014445

10.0	8.0	7.0	F1P-HA-47-10TP-S	BCD014446
		9.0	F1P-HA-47-10TP-M	BCD014447
		11.0	F1P-HA-47-10TP-L	BCD014448

12.0	10.0	7.0	F1P-HA-47-12TP-S	BCD014449
		9.0	F1P-HA-47-12TP-M	BCD014450
		11.0	F1P-HA-47-12TP-L	BCD014451

14.0	12.0	7.0	F1P-HA-47-14TP-S	BCD014452
		9.0	F1P-HA-47-14TP-M	BCD014453
		11.0	F1P-HA-47-14TP-L	BCD014454

Length = (Intrabony Length)

Surface Treatment **HA**  
Hydroxyapatite Coating

HA


A0

INSTRUMENTS

FINESIA 1P

# 1P HA ST

Straight type

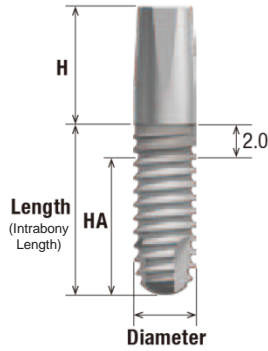

Diameter		$\phi 3.7$			Unit: mm
Length	HA	H	Product Name	Product Code	
6.0	4.0	7.0	F1P-HA-37-6ST-S	BCD014300	
		9.0	F1P-HA-37-6ST-M	BCD014301	
		11.0	F1P-HA-37-6ST-L	BCD014302	
8.0	6.0	7.0	F1P-HA-37-8ST-S	BCD014303	
		9.0	F1P-HA-37-8ST-M	BCD014304	
		11.0	F1P-HA-37-8ST-L	BCD014305	
10.0	8.0	7.0	F1P-HA-37-10ST-S	BCD014306	
		9.0	F1P-HA-37-10ST-M	BCD014307	
		11.0	F1P-HA-37-10ST-L	BCD014308	
12.0	10.0	7.0	F1P-HA-37-12ST-S	BCD014309	
		9.0	F1P-HA-37-12ST-M	BCD014310	
		11.0	F1P-HA-37-12ST-L	BCD014311	
14.0	12.0	7.0	F1P-HA-37-14ST-S	BCD014312	
		9.0	F1P-HA-37-14ST-M	BCD014313	
		11.0	F1P-HA-37-14ST-L	BCD014314	

Length = (Intrabony Length)




Surface Treatment **HA**  
Hydroxyapatite Coating

Implant

# 1P HA ST

Straight type

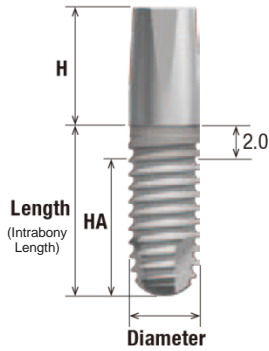

Diameter		$\phi 4.2$			Unit: mm
Length	HA	H	Product Name	Product Code	
6.0	4.0	7.0	F1P-HA-42-6ST-S	BCD014320	
		9.0	F1P-HA-42-6ST-M	BCD014321	
		11.0	F1P-HA-42-6ST-L	BCD014322	
8.0	6.0	7.0	F1P-HA-42-8ST-S	BCD014323	
		9.0	F1P-HA-42-8ST-M	BCD014324	
		11.0	F1P-HA-42-8ST-L	BCD014325	
10.0	8.0	7.0	F1P-HA-42-10ST-S	BCD014326	
		9.0	F1P-HA-42-10ST-M	BCD014327	
		11.0	F1P-HA-42-10ST-L	BCD014328	
12.0	10.0	7.0	F1P-HA-42-12ST-S	BCD014329	
		9.0	F1P-HA-42-12ST-M	BCD014330	
		11.0	F1P-HA-42-12ST-L	BCD014331	
14.0	12.0	7.0	F1P-HA-42-14ST-S	BCD014332	
		9.0	F1P-HA-42-14ST-M	BCD014333	
		11.0	F1P-HA-42-14ST-L	BCD014334	

Length = (Intrabony Length)


HA  
A0  
INSTRUMENTS  
FINESIA 1P



Surface Treatment **HA**  
Hydroxyapatite Coating

# 1P HA ST

Straight type

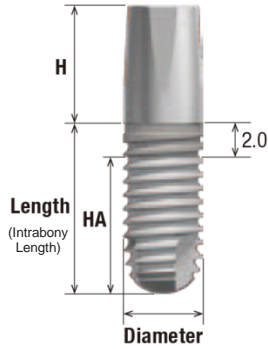

Diameter		$\phi 4.7$			Unit: mm
Length	HA	H	Product Name	Product Code	
6.0	4.0	7.0	F1P-HA-47-6ST-S	BCD014338	
		9.0	F1P-HA-47-6ST-M	BCD014339	
		11.0	F1P-HA-47-6ST-L	BCD014340	
8.0	6.0	7.0	F1P-HA-47-8ST-S	BCD014341	
		9.0	F1P-HA-47-8ST-M	BCD014342	
		11.0	F1P-HA-47-8ST-L	BCD014343	
10.0	8.0	7.0	F1P-HA-47-10ST-S	BCD014344	
		9.0	F1P-HA-47-10ST-M	BCD014345	
		11.0	F1P-HA-47-10ST-L	BCD014346	
12.0	10.0	7.0	F1P-HA-47-12ST-S	BCD014347	
		9.0	F1P-HA-47-12ST-M	BCD014348	
		11.0	F1P-HA-47-12ST-L	BCD014349	
14.0	12.0	7.0	F1P-HA-47-14ST-S	BCD014350	
		9.0	F1P-HA-47-14ST-M	BCD014351	
		11.0	F1P-HA-47-14ST-L	BCD014352	


Length = (Intrabony Length)



Surface Treatment **HA**  
Hydroxyapatite Coating

# 1P AO TP

Tapered type

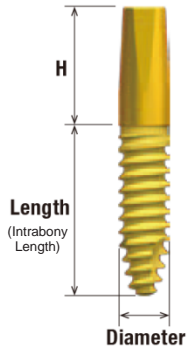

## $\phi$ 3.0 Unit: mm


Length	H	Product Name	Product Code
8.0	7.0	F1P-AO-30-8TP-S	BCD014140
	9.0	F1P-AO-30-8TP-M	BCD014141
	11.0	F1P-AO-30-8TP-L	BCD014142
10.0	7.0	F1P-AO-30-10TP-S	BCD014143
	9.0	F1P-AO-30-10TP-M	BCD014144
	11.0	F1P-AO-30-10TP-L	BCD014145
12.0	7.0	F1P-AO-30-12TP-S	BCD014146
	9.0	F1P-AO-30-12TP-M	BCD014147
	11.0	F1P-AO-30-12TP-L	BCD014148
14.0	7.0	F1P-AO-30-14TP-S	BCD014149
	9.0	F1P-AO-30-14TP-M	BCD014150
	11.0	F1P-AO-30-14TP-L	BCD014151

## $\phi$ 3.2 Unit: mm

Length	H	Product Name	Product Code
8.0	7.0	F1P-AO-32-8TP-S	BCD014160
	9.0	F1P-AO-32-8TP-M	BCD014161
	11.0	F1P-AO-32-8TP-L	BCD014162
10.0	7.0	F1P-AO-32-10TP-S	BCD014163
	9.0	F1P-AO-32-10TP-M	BCD014164
	11.0	F1P-AO-32-10TP-L	BCD014165
12.0	7.0	F1P-AO-32-12TP-S	BCD014166
	9.0	F1P-AO-32-12TP-M	BCD014167
	11.0	F1P-AO-32-12TP-L	BCD014168
14.0	7.0	F1P-AO-32-14TP-S	BCD014169
	9.0	F1P-AO-32-14TP-M	BCD014170
	11.0	F1P-AO-32-14TP-L	BCD014171

Length = (Intrabony Length)

HA  
AO  
INSTRUMENTS  
FINESIA 1P







# **INSTRUMENTS**

# Instruments

A0

HA

INSTRUMENTS


FINESIA 1P

## MARKING BUR

Used for marking the location of implant insertion

Product Name	Product Code
MARKING BUR-M	BCDI11001

Unit: mm




## PILOT DRILL 16

Creates pilot hole.

L1	L2	Color Code	Product Name	Product Code
34.5	18.0		PILOT DRL16-S	BCDI11002
38.5	22.0	●	PILOT DRL16-M	BCDI11003

Unit: mm

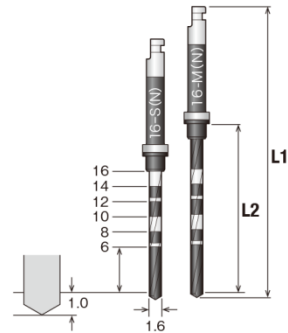


## PILOT DRILL STOPPER 16

Attached to pilot drill 16 to adjust the depth of pilot hole for implant

L	Color Code	Product Name	Product Code
5.0		PD STOPPER16-5	BCDI11010
6.0		PD STOPPER16-6	BCDI11011
7.0		PD STOPPER16-7	BCDI11012
8.0		PD STOPPER16-8	BCDI11013
9.0	●	PD STOPPER16-9	BCDI11014
10.0		PD STOPPER16-10	BCDI11015
11.0		PD STOPPER16-11	BCDI11016
12.0		PD STOPPER16-12	BCDI11017

(Including one piece)

Unit: mm

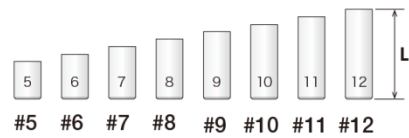


## TRIAL PIN

Used to check the depth and direction of the drilled pilot hole

L	Product Name	Product Code
18.8	TRIAL PIN16-S	BCDI11140
24.8	TRIAL PIN16-M	BCDI11141

Unit: mm




## PILOT DRILL 22

Creates pilot hole.

L1	L2	Color Code	Product Name	Product Code
34.5	18.0	●	PILOT DRL22-S	BCDI11004
38.5	22.0		PILOT DRL22-M	BCDI11005

Unit: mm

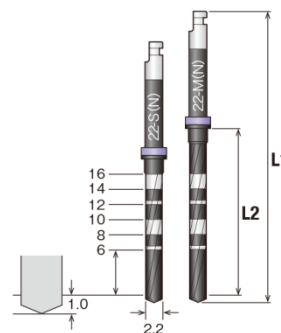


## PILOT DRILL STOPPER 22

Attached to pilot drill 22 to adjust the depth of pilot hole for implant

L	Color Code	Product Name	Product Code
5.0	●	PD STOPPER22-5	BCDI11018
6.0		PD STOPPER22-6	BCDI11019
7.0		PD STOPPER22-7	BCDI11020
8.0		PD STOPPER22-8	BCDI11021
9.0		PD STOPPER22-9	BCDI11022
10.0		PD STOPPER22-10	BCDI11023
11.0		PD STOPPER22-11	BCDI11024
12.0		PD STOPPER22-12	BCDI11025





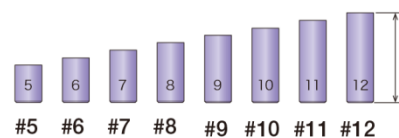

Unit: mm

(Including one piece)





## FINAL DRILL TP

Once the pilot hole is created, it is used to sequentially expand the pilot hole to achieve the final shape.





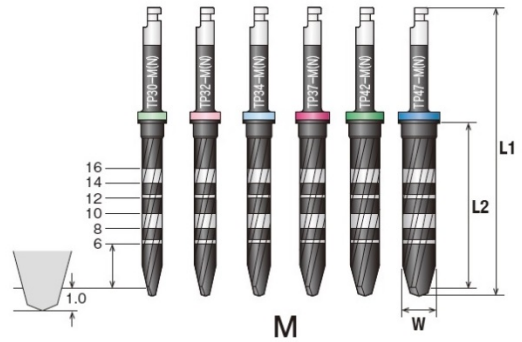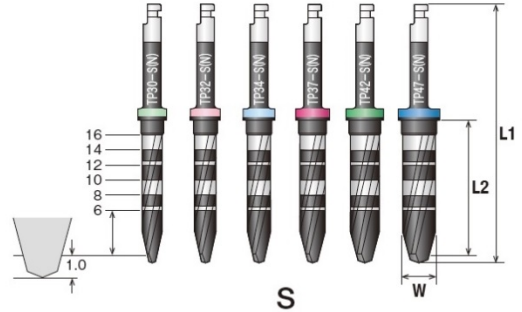

L1	L2	W	Color Code	Product Name	Product Code
S:34.4 M:38.4	S:18.0 M:22.0	2.7		FINAL DRL30-TP-S FINAL DRL30-TP-M	BCDI11030 BCDI11031
S:34.4 M:38.4	S:18.0 M:22.0	2.9		FINAL DRL32-TP-S FINAL DRL32-TP-M	BCDI11032 BCDI11033
S:34.4 M:38.4	S:18.0 M:22.0	3.1		FINAL DRL34-TP-S FINAL DRL34-TP-M	BCDI11034 BCDI11035
S:34.4 M:38.4	S:18.0 M:22.0	3.4		FINAL DRL37-TP-S FINAL DRL37-TP-M	BCDI11036 BCDI11037
S:34.4 M:38.4	S:18.0 M:22.0	3.9		FINAL DRL42-TP-S FINAL DRL42-TP-M	BCDI11038 BCDI11039
S:34.4 M:38.4	S:18.0 M:22.0	4.4		FINAL DRL47-TP-S FINAL DRL47-TP-M	BCDI11040 BCDI11041

Unit: mm





## FINAL DRILL ST

Once the pilot hole is created, it is used to sequentially expand the pilot hole to achieve the final shape.





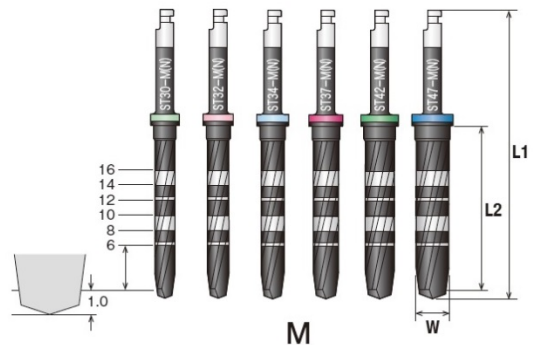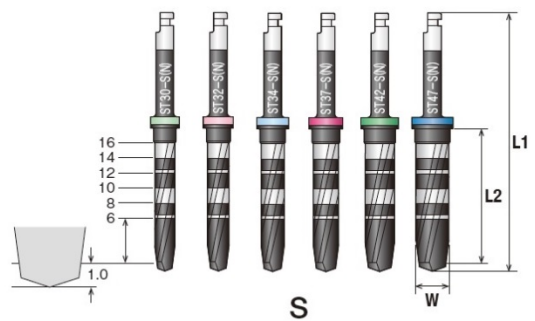

L1	L2	W	Color Code	Product Name	Product Code
S:34.4 M:38.4	S:18.0 M:22.0	2.7		FINAL DRL30-ST-S FINAL DRL30-ST-M	BCDI11050 BCDI11051
S:34.4 M:38.4	S:18.0 M:22.0	2.9		FINAL DRL32-ST-S FINAL DRL32-ST-M	BCDI11052 BCDI11053
S:34.4 M:38.4	S:18.0 M:22.0	3.1		FINAL DRL34-ST-S FINAL DRL34-ST-M	BCDI11054 BCDI11055
S:34.4 M:38.4	S:18.0 M:22.0	3.4		FINAL DRL37-ST-S FINAL DRL37-ST-M	BCDI11056 BCDI11057
S:34.4 M:38.4	S:18.0 M:22.0	3.9		FINAL DRL42-ST-S FINAL DRL42-ST-M	BCDI11058 BCDI11059
S:34.4 M:38.4	S:18.0 M:22.0	4.4		FINAL DRL47-ST-S FINAL DRL47-ST-M	BCDI11060 BCDI11061


Unit: mm




# FINAL DRILL STOPPER

Attached to the final drill to adjust the depth of implant hole


L	Color Code	Product Name	Product Code
5.0		FD STOPPER30-5	BCDI11080
6.0		FD STOPPER30-6	BCDI11081
7.0		FD STOPPER30-7	BCDI11082
8.0		FD STOPPER30-8	BCDI11083
9.0		FD STOPPER30-9	BCDI11084
10.0		FD STOPPER30-10	BCDI11085
11.0		FD STOPPER30-11	BCDI11086
12.0		FD STOPPER30-12	BCDI11087
<hr/>			
5.0		FD STOPPER32-5	BCDI11088
6.0		FD STOPPER32-6	BCDI11089
7.0		FD STOPPER32-7	BCDI11090
8.0		FD STOPPER32-8	BCDI11091
9.0		FD STOPPER32-9	BCDI11092
10.0		FD STOPPER32-10	BCDI11093
11.0		FD STOPPER32-11	BCDI11094
12.0		FD STOPPER32-12	BCDI11095
<hr/>			
5.0		FD STOPPER34-5	BCDI11096
6.0		FD STOPPER34-6	BCDI11097
7.0		FD STOPPER34-7	BCDI11098
8.0		FD STOPPER34-8	BCDI11099
9.0		FD STOPPER34-9	BCDI11100
10.0		FD STOPPER34-10	BCDI11101
11.0		FD STOPPER34-11	BCDI11102
12.0		FD STOPPER34-12	BCDI11103
<hr/>			
5.0		FD STOPPER37-5	BCDI11104
6.0		FD STOPPER37-6	BCDI11105
7.0		FD STOPPER37-7	BCDI11106
8.0		FD STOPPER37-8	BCDI11107
9.0		FD STOPPER37-9	BCDI11108
10.0		FD STOPPER37-10	BCDI11109
11.0		FD STOPPER37-11	BCDI11110
12.0		FD STOPPER37-12	BCDI11111
<hr/>			
5.0		FD STOPPER42-5	BCDI11112
6.0		FD STOPPER42-6	BCDI11113
7.0		FD STOPPER42-7	BCDI11114
8.0		FD STOPPER42-8	BCDI11115
9.0		FD STOPPER42-9	BCDI11116
10.0		FD STOPPER42-10	BCDI11117
11.0		FD STOPPER42-11	BCDI11118
12.0		FD STOPPER42-12	BCDI11119
<hr/>			
5.0		FD STOPPER47-5	BCDI11120
6.0		FD STOPPER47-6	BCDI11121
7.0		FD STOPPER47-7	BCDI11122
8.0		FD STOPPER47-8	BCDI11123
9.0		FD STOPPER47-9	BCDI11124
10.0		FD STOPPER47-10	BCDI11125
11.0		FD STOPPER47-11	BCDI11126
12.0		FD STOPPER47-12	BCDI11127

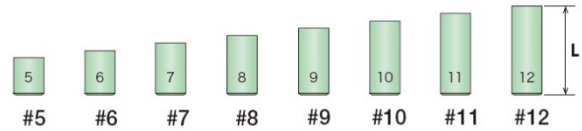


30

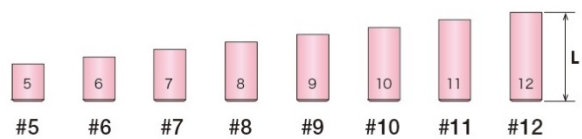


32

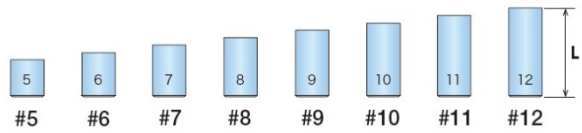


34

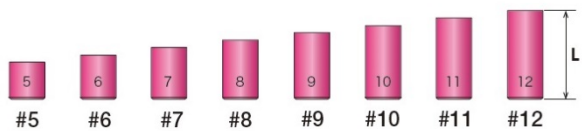

37

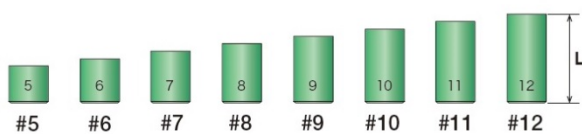

42

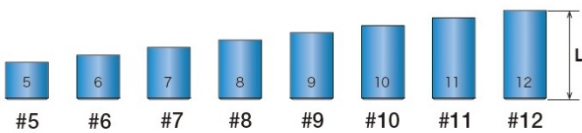

47

(Including one piece)


Unit: mm

## TRIAL GUIDE TP

Used for trial after the final shape of the implant hole is achieved

L	Product Name	Product Code
1.0	TRIAL GUIDE-TP-30	BCDI11150
	TRIAL GUIDE-TP-32	BCDI11151
	TRIAL GUIDE-TP-34	BCDI11152
0.9	TRIAL GUIDE-TP-37	BCDI11153
	TRIAL GUIDE-TP-42	BCDI11154
	TRIAL GUIDE-TP-47	BCDI11155

Unit: mm

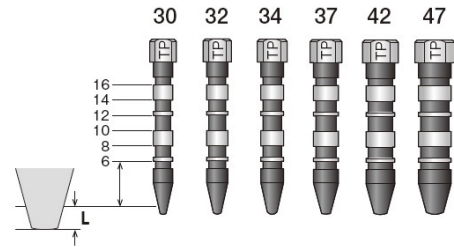


## TRIAL GUIDE ST

Used for trial after the final shape of the implant hole is achieved

L	Product Name	Product Code
0.8	TRIAL GUIDE-ST-37	BCDI11163
	TRIAL GUIDE-ST-42	BCDI11164
	TRIAL GUIDE-ST-47	BCDI11165

Unit: mm




## TAP FORMER TP

In the case of hard bone, it forms a tap according to the implant diameter.

W	Product Name	Product Code
2.9	TAP FORMER-TP-30	BCDI11180
3.1	TAP FORMER-TP-32	BCDI11181
3.3	TAP FORMER-TP-34	BCDI11182
3.6	TAP FORMER-TP-37	BCDI11183
4.1	TAP FORMER-TP-42	BCDI11184
4.6	TAP FORMER-TP-47	BCDI11185

Unit: mm

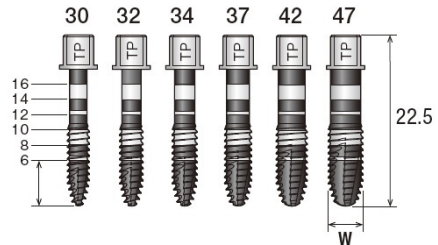


## TAP FORMER ST

In the case of hard bone, it forms a tap according to the implant diameter.

W	Product Name	Product Code
3.6	TAP FORMER-ST-37	BCDI11193
4.1	TAP FORMER-ST-42	BCDI11194
4.6	TAP FORMER-ST-47	BCDI11195

Unit: mm




## DRILL EXTENDER

Attached and used if the adjacent teeth interfere with the instruments attached to the contra-angle handpiece or if the vertical dimension is insufficient.

Product Name	Product Code
DRL EXTENDER	BCDI11235

Unit: mm






## HEXALOBULAR DRIVER CH

Attached to contra-angle handpiece or CH adapter for use, and used for transport coupling of various caps and screws

L	Product Name	Product Code
16.0	HEXALO DRIVER-XS-CH	BCDI11240
20.0	HEXALO DRIVER-S-CH	BCDI11241
24.0	HEXALO DRIVER-M-CH	BCDI11242
28.0	HEXALO DRIVER-L-CH	BCDI11243

Unit: mm

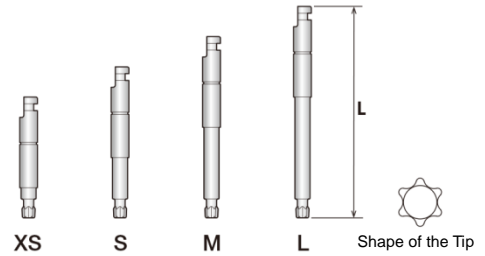


## HEXALOBULAR DRIVER SH

Used for transport coupling of various caps and screws

L	Product Name	Product Code
4.0	HEXALO DRIVER-XS-SH	BCDI11244
8.0	HEXALO DRIVER-S-SH	BCDI11245
12.0	HEXALO DRIVER-M-SH	BCDI11246
16.0	HEXALO DRIVER-L-SH	BCDI11247

Unit: mm

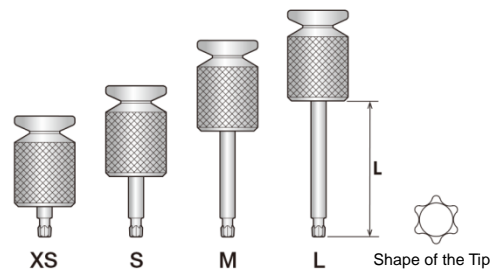


## HEXALOBULAR DRIVER WH

Attached to DA adapter or driver holder for use. Used for transport coupling of various caps and screws

L	Product Name	Product Code
4.5	HEXALO DRIVER-XS-WH	BCDI11248
6.5	HEXALO DRIVER-S-WH	BCDI11249
8.5	HEXALO DRIVER-M-WH	BCDI11250
12.5	HEXALO DRIVER-L-WH	BCDI11251

Unit: mm

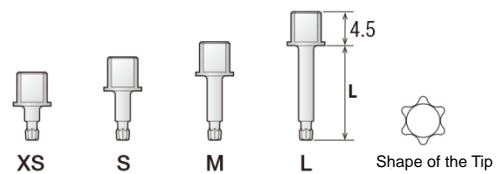

A0  
HA  
INSTRUMENTS  
FINESIA TP

## IMPLANT DRIVER

Used for final insertion of 1P implant

W	Product Name	Product Code
4.6	F1P-I DRIVER-30	BCDI11330
4.8	F1P-I DRIVER-32	BCDI11331
5.0	F1P-I DRIVER-34	BCDI11332
5.3	F1P-I DRIVER-37	BCDI11333
5.8	F1P-I DRIVER-42	BCDI11334
6.3	F1P-I DRIVER-47	BCDI11335

Unit: mm




## TORQUE WRENCH

Attached to DA adapter, CH adapter or FD adapter and used to insert the implant. Used for checking the implant insertion torque

Product Name	Product Code
TORQUEWRENCH	BCDI11286

Unit: mm

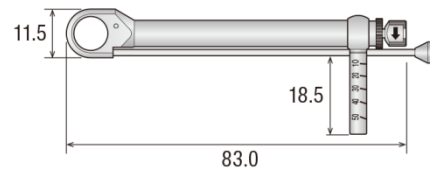


## FD ADAPTER

Attached to torque wrench

Product Name	Product Code
FD ADAPTER	BCDI11289

Unit: mm




## DA ADAPTER

Attached to torque wrench and various types of driver WH for use

Product Name	Product Code
DA ADAPTER	BCDI11287

Unit: mm

\* A separate driver holder C ring is necessary.




## CH ADAPTER

Attached to torque wrench, hexalobular driver CH for use

Product Name	Product Code
CH ADAPTER	BCDI11288

Unit: mm





## TORQUE WRENCH SET

A set comprising torque wrench and DA adapter

Product Name	Product Code
TORQUE WRENCH SET	BCDI11290

Unit: mm

\*A separate driver holder C ring is necessary.

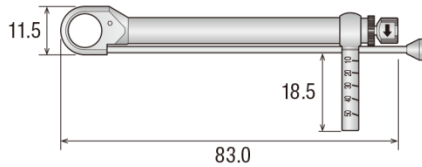


## DRIVER HOLDER

Attached to hexalobular driver WH for use

Product Name	Product Code
DRIVER HOLDER	BCDI11295

Unit: mm




## DRIVER EXTENDER

If adjacent teeth interfere during insertion of the implant, this can be attached to the DA adapter or driver holder to ensure an adequate vertical dimension.

Product Name	Product Code
DRIVER EXTENDER	BCDI11296

Unit: mm




## DRIVER HOLDER C

Attached to contra-angle handpiece and used to insert the implant

H	Product Name	Product Code
21.1	DRIVER HOLDER C-S	BCDI11275
29.1	DRIVER HOLDER C-L	BCDI11276

Unit: mm

(Including 10 pieces of driver holder C rings)



## DRIVER HOLDER C RING

Attached to driver holder C for use

Product Name	Product Code
DRIVER HOLDER C RING	BCDI11277

Unit: mm

(Including 30 pieces)



## STOPPER PICK-UP

Used to retain the final drill stopper and transport it.



Product Name	Product Code
F-STOPPER PICK UP	BCDI12005



## SURGICAL CASE

Instruments for ST- or TP-type BL, TL, or 1P can be stored.



Product Name	Product Code
F-SURGICAL CASE	BCDI12000

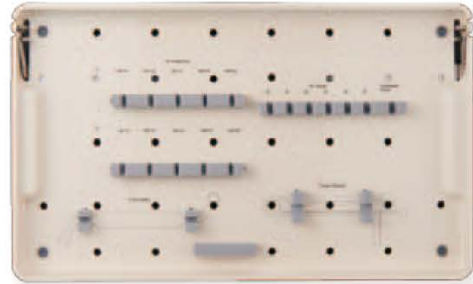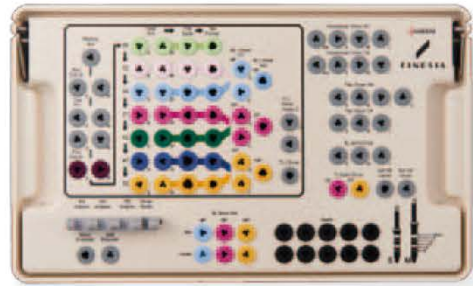

## SURGICAL CASE S

Frequently used instruments can be selected and stored.


Product Name	Product Code
F-SURGICAL CASE-S	BCDI12001



## PROSTHETIC CASE

Instruments used for secondary operations and subsequent steps can be stored.

Product Name	Product Code
F-PROSTHETIC CASE	BCDI12003



## STOPPER CASE

All sizes of stoppers can be stored, which facilitates selection and use of appropriate sizes.

Product Name	Product Code
F-STOPPER CASE	BCDI12002





## NOTES

A series of 20 horizontal dotted lines for writing notes.



# NOTES

A series of 20 horizontal dotted lines for writing notes.

FINESIA is a registered trademark of KYOCERA Corporation.

The information included in this catalog is as of August 2017.  
Reproducing or copying this catalog, in whole or in part, without  
permission is prohibited.